



SPECTRASHOP™

VERSION 6.0.0

ROBIN MYERS IMAGING

©Copyright 2020 Robin D. Myers, All Rights Reserved Worldwide

Introduction	8
System Requirements	9
Macintosh	9
Windows	9
SpectraShop™ Organization	10
Opening SpectraShop	11
Collection Window	11
Opening a Collection	12
Opening Older SpectraShop Collections	12
Specimen List.....	13
Sorting the List	13
Editing the List	13
Deleting Specimens.....	13
Adjusting the List Columns	14
Copying Specimens Between Collections	14
Saving a Spectral Graph.....	14
Printing a Spectral Graph.....	15
Specimen Reports	15
Instant Difference.....	16
Instant Average	17
Collection Window Properties.....	18
Graph Properties	18
Colorimetry	19
Colorimetric Properties	23
Patch Properties.....	25
Specimen List Properties.....	25
Editing Existing Specimens.....	26
Spectral Data.....	26
Specimen Information.....	26
Measurement Information	27
Entering New Specimens	28
Data Editor	28
Measuring.....	29
Instrument Window.....	29
Step 1. Choose an Instrument	29
Step 2. Select Connection Options (Device Dependent)	30
Step 3. Connect to the Instrument	30
Step 4. Select Specimen Type	30
Step 5. Select Instrument Options	30
Step 6. Calibrate	31
Measuring Specimens	32
Common Measurement Information	32
Measure Emissive-Light Specimens	33
Measure Emissive-Flash Specimens.....	34
Measure Emissive-Monitor Specimens	35
Auto Naming	35

Measurement	35
RGB Patch	36
Measure Reflective Specimens	37
Step 1: Set up the Auto Naming. (optional)	37
Step 2: Fill in the specimen information. (optional, but recommended)	37
Step 3: Set the measurement options. (optional)	37
Step 4: Select specimen routing. (optional)	37
Step 5: Start measuring.....	37
Measure Transmissive Specimens	40
Step 1: Set up the Auto Naming. (optional)	40
Step 2: Fill in the specimen information. (optional, but recommended)	40
Step 3: Set the measurement options. (optional)	40
Step 4: Select specimen routing. (optional).....	40
Step 5: Start measuring.	40
Measure Charts.....	42
Measure Emissive-Monitor Charts	42
Step 1: Open a chart file (required)	42
Step 2: Enter monitor information (optional, but recommended)	42
Step 3: Select measurement options (optional)	42
Step 4: Start Measuring.....	42
Measure Reflective Charts	44
Step 1: Open a chart file (required)	44
Step 2: Enter chart information (optional)	44
Step 3: Select measurement parameters (optional)	44
Step 4: Measure each patch	44
Measure Transmissive Charts.....	45
Step 1: Open a chart file (required)	45
Step 2: Enter chart information (optional)	45
Step 3: Select measurement parameters (optional)	45
Step 4: Measure each patch	45
Create a Chart	46
Emissive-Monitor Chart	46
Automatically created charts	46
Manually created charts	46
Editing a chart.....	46
Reflective Chart	48
Rectangular Chart	48
Arbitrary Chart	48
Transmissive Chart	50
Rectangular Chart	50
Arbitrary Chart	50
Graph Tool.....	51
Overview	51
Groups	51
Creating Groups.....	51
Renaming Groups	51
Adding to a Group	51

Saving a Graph	51
Printing a Graph	52
Graph 2D Properties	52
Graph Properties	52
Group Properties	53
Graph Examples	54
Locus Properties	56
Lighting Tool	57
CRI	57
TM-30-18	57
Spectral Graph.....	58
Color Vector Graph (CVG).....	58
Sample Color Fidelity (Rces) Graph	58
Local Chroma Shift (Rcs)	58
Local Hue Shift (Rhs).....	58
Local Color Fidelity (Rf).....	59
Note.....	59
TM-30 Reports.....	59
Calculator Tool	60
Add	61
Subtract	61
Multiply	61
Divide.....	61
Average.....	61
Normalize.....	61
Scale by	62
Difference Tool.....	63
Comparison Methods	63
Single Reference Comparison.....	63
Paired Comparisons.....	63
Difference Graph	63
Saving a Spectral Graph.....	63
Printing a Spectral Difference Graph.....	64
Exporting Difference Data	64
Difference Properties	65
Difference Graph Properties.....	65
Colorimetric Properties	66
Graph Properties	66
Spectral Search Tool	67
Spectral Search Properties	67
Create Light source Tool.....	68
Type	68
Initial CCT	69
Increment.....	69
Quantity to Create.....	69
Import.....	70

Supported formats.....	70
CGATS 17	70
ColorMunki.....	70
MeasureTool	70
SOCS	71
SpectraShop 1, 2, 3, 5.....	71
Spectro 1, Spectro 1 Pro	71
Spreadsheet Data, Horizontal	71
StellarNet	71
PR-655/PR-670	71
Export.....	73
Supported formats.....	73
Preferences.....	75
Collection Preferences	75
Spectral Graph.....	75
Colorimetry	76
Graph 2D Preferences	78
Graph.....	78
Difference Preferences	79
Spectral Graph.....	79
Difference Chart.....	79
Colorimetry	79
Thresholds.....	80
Search Preferences	81
Search Tolerance	81
Spectral Graph	81
Miscellaneous Preferences	82
PR-655/670 Reference White Calibration.....	82
Light Source Threshold	82
Monitor	82
Reports Preferences.....	83
Saving Preferences	83
Appendix A - Supported Instruments.....	84
Directly Supported Instruments	84
X-Rite ColorEye® XTH.....	85
Minolta FD-7	86
UV Cut Reflective Measurements.....	86
Emissive-light Measurements	86
X-Rite i1Pro1, i1Pro2, i1Pro3	87
i1Pro Variations.....	87
i1Pro Filters	87
Measurement Modes	88
Photo Research PR-655 & PR-670	89
X-Rite Spectrolino	90
Spectrolino Filters	90
Appendix B – Chart Definition File Format.....	92
Required keywords for all chart types	92

Required keywords for XY table charts.....	93
Optional keywords	94
Chart Example 1, Emissive-monitor	95
Chart Example 2, Reflective	96
Appendix C – SpectraShop 6 Import/Export Text Format	98
File Structure.....	98
File Section Keywords	99
Metadata Section Keywords.....	99
Data Format Keywords.....	100
Specimen Data Keywords.....	103
Keyword Parameters.....	103
Parameter and Data Values.....	103
Items Requiring New Metadata Section Definition.....	104
Example 1.....	106
Example 2.....	108
Appendix D – Spreadsheet Import/Export Format	113
Appendix E – Converting SpectraShop 1 and 2 Files.....	114
Specimen Type.....	114
Date Format.....	114
Appendix F – Spectral Data	115
Range	115
Sampling	116
Appendix G – Frequently Asked Questions (FAQ).....	117
References.....	118
Standards.....	118
Books	119
Papers	120

INTRODUCTION

SpectraShop™ is a powerful set of tools for measuring, storing, organizing and analyzing visible light spectra.

SpectraShop™ does:

- Measure emissive, reflective and transmissive spectra directly from spectrometers
- Create collections of spectra
- Calculate colorimetric and densitometric values
- Measure monitor, print and transparency charts
- Import spectral data from other programs or instruments
- Export spectral data for use in other programs
- Convert spectral data between file formats
- Create graphs of colorimetric and densitometric values
- Calculate color differences with threshold Pass/Fail indications
- Analyze lighting with TM-30-18 and CRI
- Combine spectra mathematically
- Produce Plankian and D-series illuminants
- Print graphs with publication quality
- Export graphs to files
- Produce PDF reports of specimens and TM-30 analysis

SpectraShop does **not**:

- Create ICC color management profiles
- Analyze ICC profiles
- Input or import colorimetric values

SYSTEM REQUIREMENTS

MACINTOSH

- Intel processor
- MacOS 10.6 or later
- 1024 x 768 or larger monitor
- One of the supported spectral measurement instruments


WINDOWS

- Windows XP or later
- 1024 x 768 or larger monitor
- One of the supported spectral measurement instruments

SPECTRASHOP™ ORGANIZATION

GENERATE DATA

Spectrometer Measurement

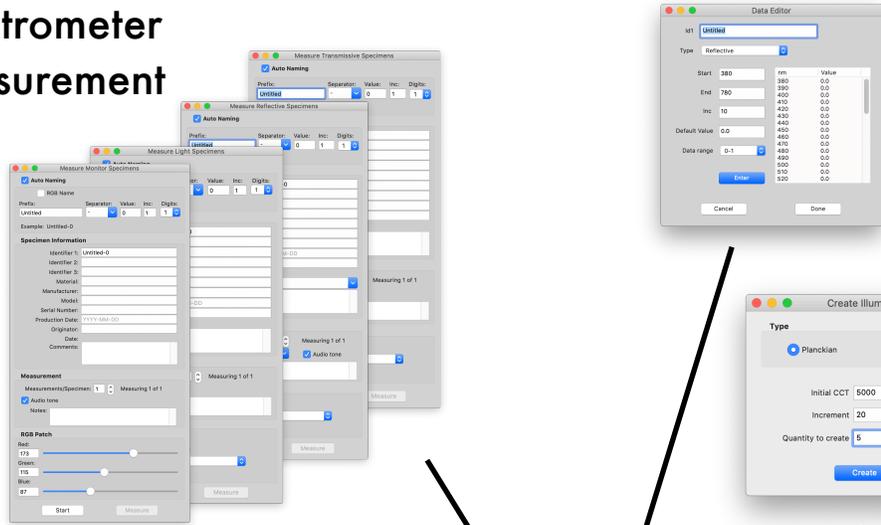


Manual Entry

Light Source Generator

STORE DATA

Collections


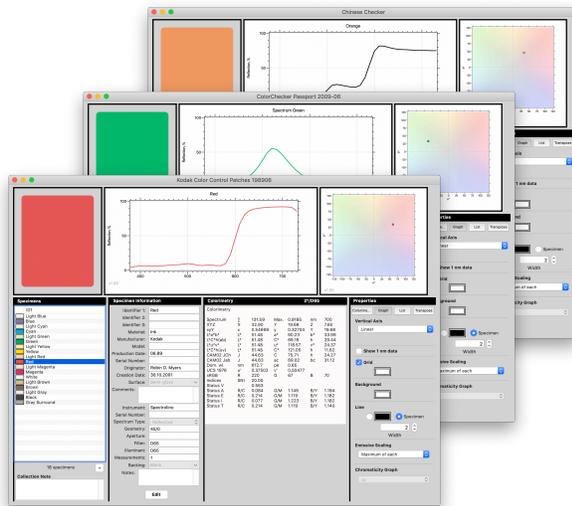


ANALYZE DATA

TM-30-18 Lighting Analysis

Find Matches

Difference

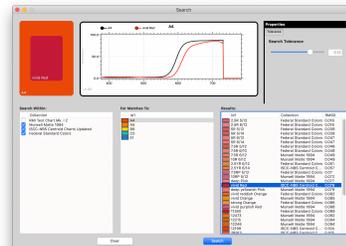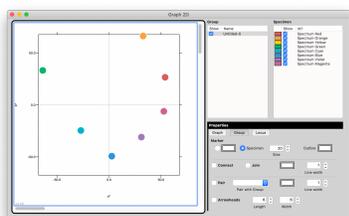


Graphical Analysis

OPENING SPECTRASHOP

When SpectraShop™ opens, a director window is displayed to provide one of the following options:

1. Open an existing spectral data file
2. Measure specimens
3. Measure charts

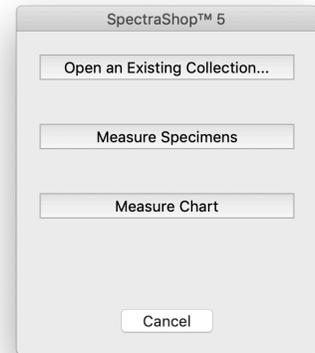


At this point, select one of the available options to begin your work.

If you are on a Macintosh computer, you may also choose to execute one of the menu commands. This ability is not available on Windows computers because of its method of handling menus.

COLLECTION WINDOW

The Collection window is the heart of SpectraShop. All the tools, operations and graphs derive from the data within collections.

A collection is a group of one or more spectra along with the associated descriptive and measurement information, known as metadata. Each spectrum and its metadata is called a *specimen*. Typically, the specimens in a collection share some common characteristics. For example, a collection might be a series of manufacturer's inks, a set of fluorescent lamps, or a group of photographic filters.

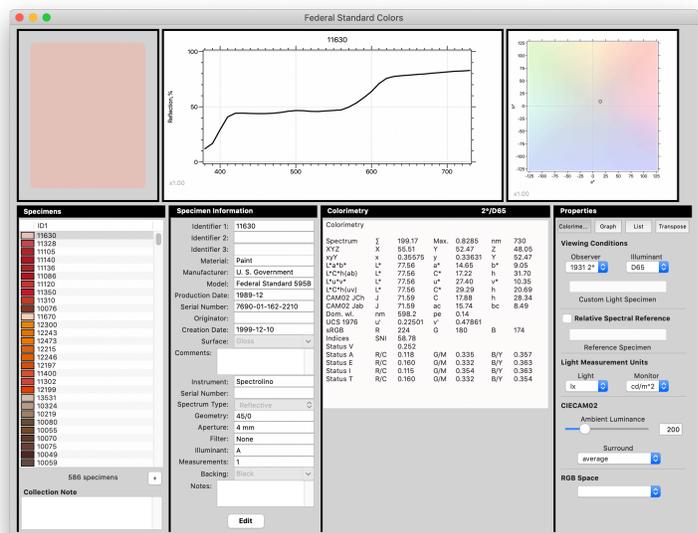

Multiple collections may be open simultaneously, limited only by your computer's memory. Having more than one collection open allows transferring data between collections, different ways to organize the data, and better operations with some of the analysis tools.


OPENING A COLLECTION

Each collection is opened and displayed in its own window using the *File/Open* menu option. The window shows a list of all the specimens in the collection. As each specimen is selected in the list its associated information is displayed in the *Specimen Information* area.

The specimen's spectrum is displayed as a graph at the top of the collection window. In the upper-right corner, an a^*b^* graph maps the position of the specimen in the a^*b^* plane.

A color patch representing the visual appearance of the spectrum is displayed to the spectral graph's immediate left.

From the spectral data color metrics are calculated then displayed in the *Colorimetry* area.

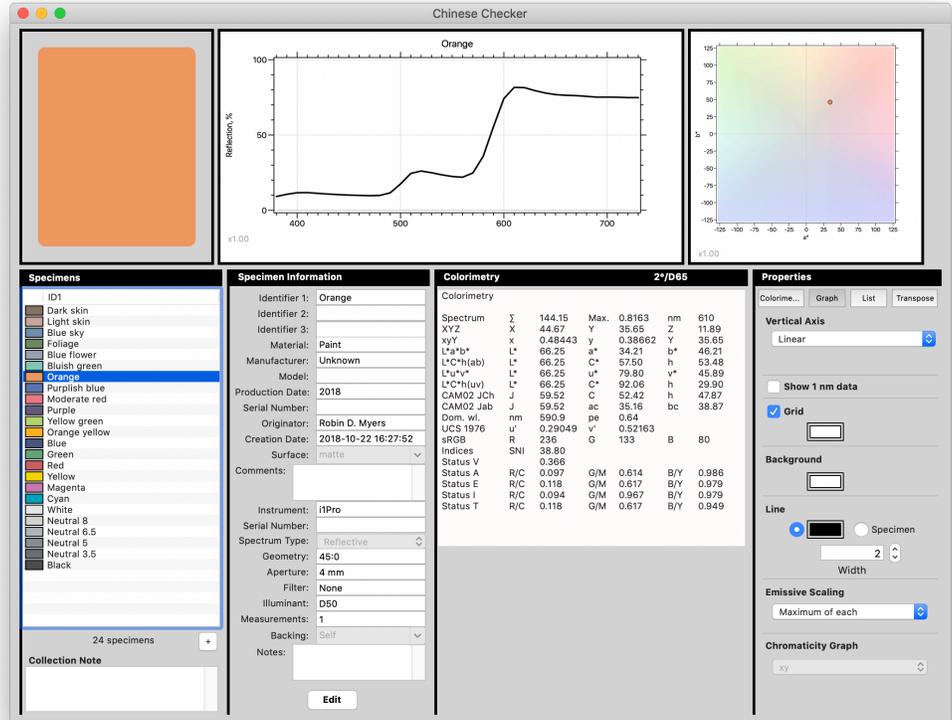

OPENING OLDER SPECTRASHOP COLLECTIONS

SpectraShop 6 will open older collections, automatically converting them as closely as possible into the version 6 format.

In versions 1 and 2 the dates were treated as simple text strings, allowing for any format. Beginning with SpectraShop 3, the ISO 8601 format of YYYY-MM-DD is used. Older date strings will need to be converted manually into the ISO format. Appendix E gives more information on converting the dates.

SPECIMEN LIST

When a collection is first opened, the *Specimens* list displays the primary identifier, *ID1*, and a color swatch representing the approximate color of the specimen. The collection specimens are listed in the order they are stored within the file.

The first specimen is automatically highlighted once the collection file has been read into the *Specimens* list. Its metadata is displayed in the *Specimen Information* area along with the details about how the specimen was acquired.

Note: It is possible to modify the *Specimens* list to show up to 8 items, either metadata or colorimetric. For details, consult the Properties chapter in the Specimens List Properties section.

SORTING THE LIST

The list can be sorted in ascending or descending alphabetic order by successively clicking on the *ID1* list column labels. A small triangle appears in the column heading to indicate the direction of the sort; ascending or descending.

Note: When a specimen list is saved, the specimens are written to the file in the order in which they appear in the collection window. Saving a sorted list will result in the file being written with the specimens in sorted order.

Numeric columns may also be used for sorting the list. For instance, if the list contains light source measurements and the CCT has been added to the list, then the list may be sorted in increasing CCT order by clicking the CCT label in the list's column heading.

After the specimen list has been sorted, it may be put back to the original order by clicking the *Unsort* button in the *List Properties* in the lower-right corner of the window.



List sorted in ascending alphabetic order

EDITING THE LIST

Specimens in the list can be manually rearranged by clicking on a specimen's identifier, then dragging the specimen to a new position. A horizontal bar will appear to show where the specimen will be placed in the list.

DELETING SPECIMENS

Specimens can be deleted from the list by highlighting the specimens to delete, then pressing the *Delete* key (Macintosh) or the *Backspace* key (Windows).

A range of items can be selected and deleted by clicking on the first specimen to delete, then holding down the *Shift* key and clicking on the last specimen to delete. The entire range will be deleted when the *Delete* key is pressed.

Non-adjacent items can be selected by holding down the *Command* key (Macintosh) or the *Control* key (Windows), then clicking on the various specimens.

Note: Before they are deleted from the list, you will be requested to confirm their deletion. This is necessary because SpectraShop does not have an Undo feature. So be careful. It is advised to save a copy of the collection before deleting any specimens.

ADJUSTING THE LIST COLUMNS

Often it is necessary to see more of the identifiers than can be shown in the space allotted to the Specimens list. There are two ways to see more. The first is to expand the width of the collection window. The Specimens list will automatically widen as the window width increases.

The second way to show more of the identifiers is to click and drag the small vertical bar between the identifier names at the top of the Specimens list.

COPYING SPECIMENS BETWEEN COLLECTIONS

Often it is necessary to put specimens from several collections into one collection. SpectraShop supports two methods for transferring specimens between collections. The first method is by means of *Drag and Drop*. It is accomplished by highlighting the specimens in the collection to copy from, then dragging the specimen to the destination collection list. When the mouse button is released over the destination list the specimens will be *copied*, not moved, to the destination collection.

The second copy method is by *Copy/Paste*. The specimens to copy may be highlighted, then copied using the *Command C* keyboard key combination (Mac) or the *Control C* keys (Windows). Then make the destination collection the topmost window, position the cursor in the destination specimen list and press the *Command V* keys (Mac) or *Control V* keys (Windows) to enter the specimens into the list.

SAVING A SPECTRAL GRAPH

The spectrum graph can be saved to a file by first clicking inside the graph to select it, indicated by a blue border (Mac) or a shimmy (Windows). Then choose the *File/Save Graph* menu command. The file format can be selected from JPEG or PNG (Mac), GIF or TIFF (Windows) in the File Save dialog window.

Note: All file types are not available on all platforms.

JPEG files are automatically saved with the maximum quality setting to help prevent any visible artifacts in the resulting image file.


PRINTING A SPECTRAL GRAPH

Spectrum graphs are created with sufficient resolution to allow for a minimum 10 inch print at a resolution of at least 300 ppi. To print the selected spectral graph, select the *File/Print* menu command. Parameters relating to the printer's page definitions may be set using the *File/Page Setup* menu command. If the page has not been defined before the *Print* command is issued, *Page Setup* will be automatically executed before the *Print* command executes.


SPECIMEN REPORTS

SpectraShop can create a *PDF report*, a file with the information contained in the collection window. To create the report, select *Create Report* from the *File* menu. The PDF file will contain a single page for each specimen until pages for all the currently selected specimens have been created.

Each PDF page may also have an optional company logo placed on the page. To select the logo file, use the *Reports* tab in the *Preferences*. The position of the logo is fixed in the report design and cannot be changed.

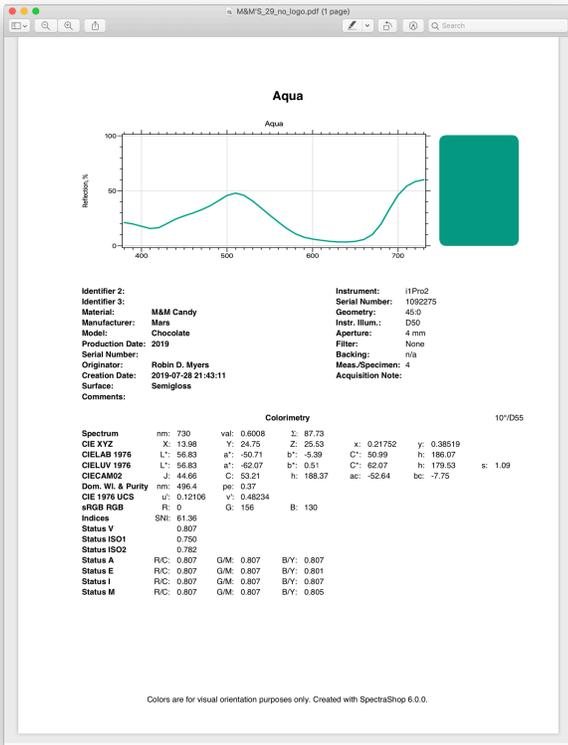

Single specimen report without a logo.

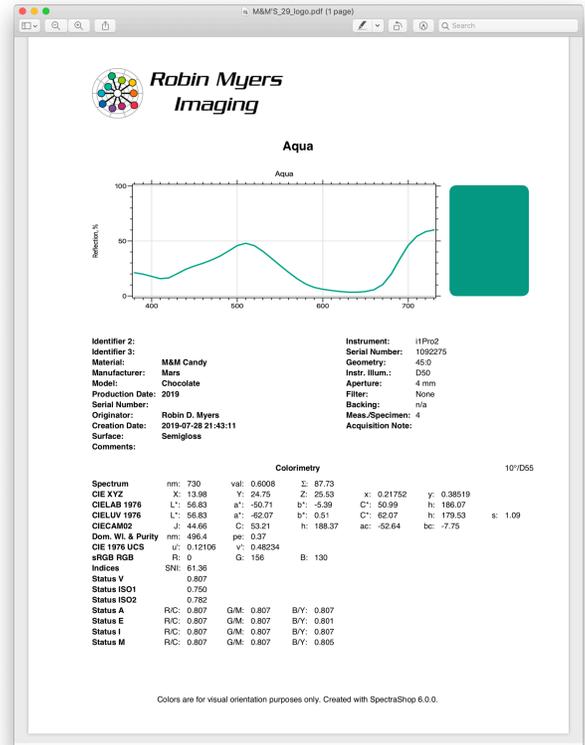

Single specimen report with a logo.

INSTANT DIFFERENCE

The colorimetric differences between two specimens may be quickly calculated by selecting two specimens in the list. The individual colorimetric difference values are displayed in the Colorimetry area with a leading Δ character to indicate the values shown are differences. In addition, the perceptual difference values for ΔE_{ab} , ΔE_{94} , ΔE_{2000} and ΔE_{CMC} are shown in the normally blank area below the *Colorimetry* display, along with RMSD, the Root Mean Square of the Difference.

Clicking on the *Append Average to List* button will calculate the spectral average of the two selected specimens and add it to the bottom of the list.

The screenshot displays the M&M'S 29 software interface. At the top, there are three panels: a color swatch of a green square with a darker green square inside labeled 'Dark Green', a spectral reflectance graph showing two curves (Green and Dark Green) from 400 to 700 nm, and a CIE color space plot with two points. Below these are four main sections: Specimens, Specimen Information, Colorimetry, and Properties.

Specimens: A list of 29 color swatches. 'Green' and 'Dark Green' are selected.

Specimen Information:

- Identifier 1: [Blank]
- Identifier 2: [Blank]
- Identifier 3: [Blank]
- Material: M&M Candy
- Manufacturer: Mars
- Model: Chocolate
- Production Date: 2019
- Serial Number: [Blank]
- Originator: Robin D. Myers
- Creation Date: 2019-07-28 21:49:54
- Surface: Semigloss
- Comments: [Blank]
- Instrument: i1Pro2
- Serial Number: 1092275
- Spectrum Type: Reflective
- Geometry: 45:0
- Aperture: 4 mm
- Filter: None
- Illuminant: D50
- Measurements: 4
- Backing: n/a
- Notes: [Blank]

Colorimetry (10°/D55):

Differences				
Spectrum	$\Delta \Sigma$	39.15		
XYZ	ΔX	-10.68	ΔY	-16.22
	ΔZ	-3.27		
xyY	Δx	-0.05209	Δy	0.01092
	ΔY	-16.22		
L*a*b*	ΔL^*	-21.13	Δa^*	1.11
	Δb^*	-18.12		
L*C*h(ab)	ΔL^*	-21.13	ΔC^*	-12.09
	Δh	-13.55		
L*u*v*	ΔL^*	-21.13	Δu^*	3.43
	Δv^*	-20.78		
L*C*hs(uv)	ΔL^*	-21.13	ΔC^*	-17.00
	Δh	12.13		
CAM02 JCh	ΔJ	-19.94	ΔC	-9.89
	ΔH	11.92		
CAM02 Jab	ΔJ	-19.94	Δac	0.69
	Δbc	-15.24		
UCS	$\Delta u'$	-0.02667	$\Delta v'$	-0.00345
SNI	ΔSNI	9.32		
Status V	ΔV	0.290		
Status A	$\Delta R/C$	0.290	$\Delta G/M$	0.290
	$\Delta B/Y$	0.290		
Status E	$\Delta R/C$	0.290	$\Delta G/M$	0.290
	$\Delta B/Y$	0.291		
Status I	$\Delta R/C$	0.290	$\Delta G/M$	0.290
	$\Delta B/Y$	0.289		
Status T	$\Delta R/C$	0.290	$\Delta G/M$	0.290
	$\Delta B/Y$	0.290		

Differences	
ΔE_{ab}	27.86
ΔE_{94}	22.58
ΔE_{2000}	21.73
ΔE_{CMC}	22.62
RMSD	0.132

Properties:

- Colorimetry | Graph | List | Transpose
- Vertical Axis: Linear
- Show 1 nm data:
- Grid:
- Background:
- Line: [Blank] Specimen
- Width: 2
- Emissive Scaling: Maximum of each
- Chromaticity Graph: xy

Buttons: Append Average to List, Edit

INSTANT AVERAGE

When 3 or more specimens are selected in the *Specimen List*, the colorimetric averages between the specimens are calculated, then displayed in the individual colorimetric Colorimetry area. All the colorimetric values change from their normal identifications to ones preceded by a μ character. Many will recognize this as the symbol for the statistical mean, or average, value.

The *Append Average to List* button is available to add the average spectrum to the bottom of the list.

The screenshot displays the M&M'S 29 software interface. At the top, the title bar reads "M&M'S 29". The main window is divided into several sections:

- Top Left:** A legend showing four color swatches: Teal, Green, Dark Green, and Electric Green.
- Top Center:** A line graph showing Reflectance (%) on the y-axis (0 to 100) versus wavelength (nm) on the x-axis (400 to 700). Four curves represent the spectra for Teal, Green, Dark Green, and Electric Green.
- Top Right:** A colorimetric graph showing the distribution of colorimetric values in a 2D space.
- Bottom Left (Specimens):** A list of 29 color swatches. The selected colors are Teal, Green, Dark Green, and Electric Green.
- Bottom Center (Specimen Information):** Fields for Identifier 1-3, Material (M&M Candy), Manufacturer (Mars), Model (Chocolate), Production Date (2019), Serial Number (1092275), Originator (Robin D. Myers), Creation Date (2019-07-28 21:45:32), Surface (Semigloss), Instrument (i1Pro2), and Spectrum Type (Reflective).
- Bottom Center-Right (Colorimetry):** A table of colorimetric averages for 10°/D55. The values are preceded by a μ character, indicating they are averages.

Averages	$\mu\Sigma$	μX	μY	μZ
Spectrum	65.29	14.83	21.03	6.83
XYZ	μX	μY	μZ	
xyY	0.31668	0.49610	21.03	
L*a*b*	μL^*	μa^*	μb^*	
L*C*h(ab)	μL^*	μC^*	μh	
L*u*v*	μL^*	μu^*	μv^*	
L*C*hs(uv)	μL^*	μC^*	μh	
CAM02 JCh	μJ	μC	μH	
CAM02 Jab	μJ	μa	μb	
UCS	$\mu u'$	$\mu v'$	$\mu w'$	
SNI	μSNI			
Status V	μV	$\mu G/M$	$\mu B/Y$	
Status A	$\mu R/C$	$\mu G/M$	$\mu B/Y$	
Status E	$\mu R/C$	$\mu G/M$	$\mu B/Y$	
Status I	$\mu R/C$	$\mu G/M$	$\mu B/Y$	
Status T	$\mu R/C$	$\mu G/M$	$\mu B/Y$	
- Bottom Right (Properties):** A panel with tabs for Colorimetry, Graph, List, and Transpose. It includes options for Vertical Axis (Linear), Show 1 nm data, Grid (checked), Background, Line (Specimen selected), Width (2), Emissive Scaling (Maximum of each), and Chromaticity Graph (xy).

An "Append Average to List" button is located at the bottom center of the Colorimetry section.

COLLECTION WINDOW PROPERTIES

Click on the *Inspector* icon to access the properties for the collection window. The properties are grouped by functionality represented by tabs at the top of the collection properties window.

Graph Properties

Data Display

For reasons explained in the *Colorimetry* section, all spectra that are not natively sampled at 1 nm intervals are interpolated by SpectraShop internally to 1 nm. The resulting 1 nm spectrum can be displayed by checking *Show 1 nm data* from the *Graph Properties* section.

The original measured data can be displayed by moving the cursor into the graph and clicking on the spectral line, holding the mouse button down. The value at each sampling interval is displayed above the graphed spectral line. When the mouse button is released, the value data display will disappear.

Grid

A grid can be displayed by checking the *Show* box. The color for the grid lines is selected by clicking in the *Color* box.

Background

The graph's background color can be selected by clicking in the associated *Color* box. This is a useful feature for improving the visibility of spectral graphs when the specimen's color is used for the line and the background color is similar to the specimen's color.

Line

This section controls the display of the specimen's line graph. The line color can be chosen to be the one in the *Color* box or the color calculated from the specimen's spectrum. When the *Specimen* color is used it is sometimes necessary to change the background color to improve the line's visibility.

Emissive-Light Scaling

Graphing emissive light spectra can present a problem for setting the scale. There can be a wide variance in the luminous flux from different sources which makes meaningful graphic comparisons problematic. SpectraShop presents a choice between *560 nm, Maximum of each* or *Maximum of all* value scaling.

When white light sources with relatively smooth spectra are displayed it is often the practice to scale the graph data so each spectrum has its 560 nm value at 1 on the graph's scale.

This may create a visual problem for sources that have 560 nm data with very low or high values in relation to the other spectra being displayed. It also does not work for non-white light sources, such as a red LED with no appreciable value at 560 nm.

When comparing monochromatic or non-white sources the *Maximum of each* option will find each specimen's maximum spectral value, using it to scale the graph to place this value at 1 on the scale. This may make darker specimens appear to be as bright as much brighter specimens, but it can make it easier to compare spectral features.

A better choice for comparing the relative magnitude of the light sources is the *Maximum of all* option. All the selected specimens are examined to find the overall maximum value, then this value is used to scale all the specimens.

Colorimetry

To be compliant with the CIE recommendations for colorimetric calculations, SpectraShop 6 converts all spectra internally to 1 nm data prior to performing colorimetric calculations. While this means that there is much more data to process, the advantage is that spectra with different sampling intervals can now be interchangeably combined, something that may be impossible with other programs.

Parameters affecting the colorimetric calculations can be selected individually for each collection from the Properties window. Click on the *Colorimetry* button at the top of the *Properties* window to access these attributes.

Depending on the type of object type being analyzed, the following values are calculated:

XYZ Tristimulus values

Standardized spectral response for the Standard Observer (a representation of a typical human observer).

xy Chromaticity values

A set of values derived from XYZ which are commonly used to produce a two-dimensional graphic representation of human color response, known as a chromaticity diagram.

u'v' Chromaticity values

A set of values derived from XYZ which produce more perceptually uniform chromaticity diagram than the xy diagram.

CIE L*a*b*C*h 1976 values

These values were derived from XYZ to make a color space where color differences are more perceptually uniform. L* corresponds to lightness, a* to redness/greenness, b* to yellowness/blueness. C* is chroma, how strong is the color. h is the hue angle in degrees. L*a*b* define a Cartesian coordinate system for color definition, L*C*h define a cylindrical coordinate system.

CIE L*u*v*C*hs 1976 values

These values were derived from the u'v' chromaticity values to make a color space where color differences are more perceptually uniform. L* corresponds to lightness (and is the same as in the L*a*b* 1976 system), u* to redness/greenness, v* to yellowness/blueness. C* is chroma, how strong is the color. h is the hue angle in degrees. s is the saturation. L*a*b* define a Cartesian coordinate system for color definition, L*C*h define a cylindrical coordinate system. This system is used for some applications instead of L*a*b*.

CIECAM02 JChab values

This is the latest attempt to create a set of color values more closely corresponding to perception than CIE L*a*b* 1976 or CIE L*u*v* 1976. J corresponds to lightness, C to chroma, and h to hue angle. The opponent color values *a* and *b* fill roles similar to the *a** and *b** opponent values of CIE L*a*b* 1976 system.

Dominant wavelength

A representation of the specimen's color calculated from the xy chromaticity diagram and expressed in nanometers. This value is calculated by projecting a line from the white point through the specimen's xy location to the spectral locus to find the wavelength. For the colors that project to the non-spectral purple line (the line connecting violet to red) the accepted convention is to express the wavelength as the negative value of the opposite green wavelength value.

Excitation purity, p_e

A representation of the specimen's colorfulness calculated from the xy chromaticity diagram. When used with the dominant wavelength and the Y value it can be used to define a color.

UCS 1976 u', v' (reflective and transmissive)

This is an older set of colorimetric values predating the CIE 1976 L*u*v* values. It is still used in evaluating some light sources.

Indices, SNI (reflective and transmissive)

The Spectral Neutrality Index (SNI) is used to evaluate the evenness of the specimen's spectrum from 380 to 780 nm, inclusive. This is very useful for comparing neutral specimens.

Indices, WI and TI (reflective)

WI and TI are CIE Whiteness and Tint Indices for paper. They are displayed only if a paper is within a very close colorimetric distance from the illuminant.

Photometry (emissive)

The amount of light flux illuminating a point is reported in lux or in W/m^2 , depending on the Properties setting.

For monitors, the light emitted from a point on the display's surface is expressed as cd/m^2 , or $W/(m^2 \cdot sr)$, depending on the Properties setting.

The Correlated Color Temperature, CCT is displayed for both emissive light and monitors as Kelvin.

RGB

The red (R), green (G) and blue (B) values for the specimen in one of the selected RGB color spaces. A chromatic adaptation transform (CAT) used to adapt the values when the viewing illuminant is different from the RGB space illuminant.

The choice of RGB space is linked to the viewing condition illuminant in SpectraShop's Preferences. It is always advised to keep the viewing illuminant and RGB space link enabled.

Visual Density (reflective and transmissive)

Used to evaluate the lightness or darkness of an image to be viewed directly (e.g. prints) or projected (e.g. black-and-white transparencies). It can be used to evaluate any material viewed by the human visual system, with or without color.

Status A Density (reflective and transmissive)

The filter responses were designed to match the characteristics of prints or films viewed directly, or projected. Examples of these materials include transparencies (reversal film) and reflective color prints.

Status E Density (reflective)

The filter responses were designed to match reflective graphics arts materials used in Europe. Used to evaluate materials such as original art, printed materials, off-press proofs and press sheets.

Status I Density (reflective)

Narrow band filter responses designed to approximate monochromatic densitometry. Used for the evaluation of process inks on paper.

Status M Density (transmissive)

Used for the evaluation of color negative film which will be printed on photographic paper but will not be viewed directly.

Status T Density (reflective)

The filter responses were designed to match reflective graphics arts materials used in the United States. Used to evaluate materials such as original art, printed materials, off-press proofs and press sheets.

Colorimetric Properties

Viewing Conditions

The observer can be selected from the CIE 1931 2° observer or the CIE 1964 10° observer.

For reflective specimens a choice of standard illuminants is offered:

A	Tungsten
C	Daylight
D50	Simulated daylight at 5000 K D55 Simulated daylight at 5500 K
D65	Simulated daylight at 6500 K D75 Simulated daylight at 7500 K
E	Equal energy
F1	Fluorescent, standard
F2	Fluorescent, standard
F3	Fluorescent, standard
F4	Fluorescent, standard
F5	Fluorescent, standard
F6	Fluorescent, standard
F7	Fluorescent, broad band
F8	Fluorescent, broad band
F9	Fluorescent, broad band
F10	Fluorescent, narrow band
F11	Fluorescent, narrow band
F12	Fluorescent, narrow band
LED-B1	Phosphor LED, Blue emitter
LED-B2	Phosphor LED, Blue emitter
LED-B3	Phosphor LED, Blue emitter
LED-B4	Phosphor LED, Blue emitter
LED-B5	Phosphor LED, Blue emitter
LED-BH1	Phosphor LED, Blue emitter, Hybrid
LED-RGB1	Phosphor LED, Red, Green and Blue emitters
LED-V1	Phosphor LED, Violet emitter
LED-V2	Phosphor LED, Violet emitter
ID50	Indoor D50, D50 filtered through window glass
ID65	Indoor D65, D65 filtered through window glass
Custom	User specified light source

When *Custom* is selected, the light source specimen in the *Custom Light Specimen* field is used for the colorimetric calculations.

Spectral Reference

Emissive-light and emissive-monitor colorimetry can be referred to a white by dragging the white specimen from the specimen list into the field to the right of the Relative checkbox. This is especially important for monitor colorimetry where the measurements need to be referenced to the monitor white. The colorimetry will be recalculated and the colorimetric values are updated with the new values. Once the reference white is defined, the Relative checkbox can be used to switch between the original values and the relative values.

Light Measurement Units

The light measurement units for emissive specimens can be selected from the appropriate popup menus.

Light: illuminance (lx) or irradiance (W/m²)

This is the amount of light impinging on a place from the light source.

Note: This value is dependent upon the distance from the light source, **it is highly recommended that this distance be measured and recorded in the *Measurement Notes* field.**

Monitor: luminance (cd/(m²) or radiance (W/(m² sr)

This is the amount of light exiting the surface of the display.

CIECAM02

The adapting field luminance is selected from the *La* field and slider. The *Surround* popup menu selects the brightness of the area surrounding the specimen.

RGB Space

The XYZ values are converted into an RGB space selected from the popup menu. By default this space is *sRGB*. It can be changed in the *Preferences* window to any of the currently supported spaces.

Note: In the current release there is no chromatic adaptation transform (aka CAT) applied to the RGB data. This means that if the currently selected RGB space has a different white point from the selected viewing illuminant, then the RGB values will not be valid.

Here is a list of the white points for the supported RGB spaces.

Adobe 1998	D65
Apple	D65
Beta	D50
CIE	E
ColorMatch	D50
eciRGB v2	D50
HDTV	D65
LCD	Custom
NTSC	C
ProPhoto	D50
SMPTE-C	D65
sRGB	D65
Wide Gamut	D50

The viewing environment white space can be set to match any of the RGB space white points except the *Custom* white point for the *LCD* space.

Note: The *LCD* space is provided to be complementary with the RGB spaces provided in Adobe Photoshop. It is not meant to be representative of any particular LCD monitor.


Patch Properties

The only patch property currently available is the color of the area surrounding the patch. For better color assessment, the patch should be a mid-tone neutral gray. Changing the surround to be more colorful allows for some interesting perceptual experiments. Click the *Patch* icon at the top of the *Properties* window to access these properties.

Specimen List Properties

List Columns

The first popup chooses the number of extra columns to display in the Specimen List. The list always shows two columns; a simulated color patch and Identifier 1. Up to 8 additional data values may be added to the list. Once the number of columns to add to the list has been chosen, select the item for each column from the corresponding popup menus. In the example on the right, one additional column showing the CCT has been added to a list of common light sources.

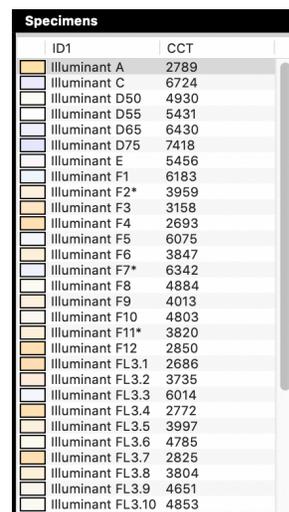

ID1	CCT
illuminant A	2789
illuminant C	6724
illuminant D50	4930
illuminant D55	5431
illuminant D65	6430
illuminant D75	7418
illuminant E	5456
illuminant F1	6183
illuminant F2*	3959
illuminant F3	3158
illuminant F4	2693
illuminant F5	6075
illuminant F6	3847
illuminant F7*	6342
illuminant F8	4884
illuminant F9	4013
illuminant F10	4803
illuminant F11*	3820
illuminant F12	2850
illuminant FL3.1	2686
illuminant FL3.2	3735
illuminant FL3.3	6014
illuminant FL3.4	2772
illuminant FL3.5	3997
illuminant FL3.6	4785
illuminant FL3.7	2825
illuminant FL3.8	3804
illuminant FL3.9	4651
illuminant FL3.10	4853

You can choose from most of the Specimen and Measurement metadata items, along with all the Colorimetry items.

Note: SpectraShop allows for mixed data type lists, thus some colorimetric items may not be supported for a specimen, depending on the Spectrum Type. When this happens the column for that particular specimen will be left blank. For example, an emissive-light specimen will not display any L^* values until the specimen is calculated in relative mode.

Unsort

When the Specimen List has been sorted by the values in one of the columns, clicking this button will return the list to the original order as it occurred in the collection file.



EDITING EXISTING SPECIMENS


SPECTRAL DATA

A specimen's spectral data may be edited by double-clicking on the specimen in the collection list. This will open the *Data Editor*.

To prevent accidentally introducing wavelength errors the data values may be edited, but not the wavelength values. Highlight any data value, type the new value, then advance to the next data value with the *Return* key, *Tab* key or the down arrow key.

To move up the list to the previous data value; type *Shift-Tab* or the up arrow key.

When finished editing the data, click the *Done* button to send the edited specimen back to the specimen list. Notice that it has the word "copy" appended to the original specimen name to prevent accidentally overwriting the original data.

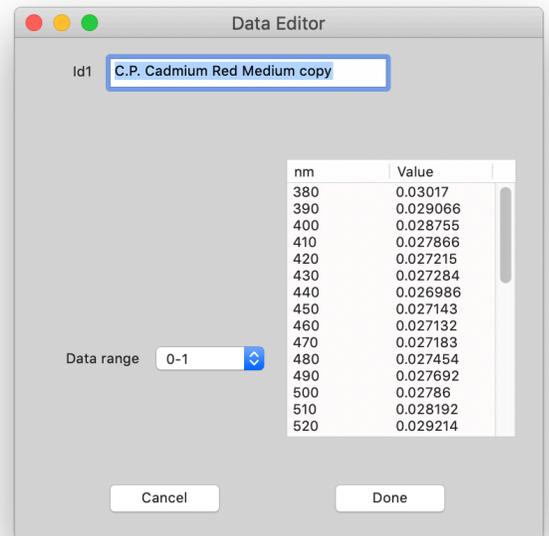

SPECIMEN INFORMATION

A specimen's descriptive information, also known as metadata, may be edited by clicking on the *Edit Metadata* icon in the top-left corner of the collection window. Entering information into the edit fields will immediately update the information in the selected specimens.

Note: SpectraShop uses the ISO 8601 date format of *YYYY-MM-DD*. Entering less than the full date is possible but the ISO 8601 format is still used. For example, entering a year and month can be entered as 1998-10, for October 1998. If only the year is known it can be entered as 1998. Entering the year as the last two digits only is not allowed. The hyphens must be present if more than the year is entered. For single digit months and days it is not necessary to enter a leading 0, the field will add it for you. For example, 2001-1-5 can be entered for 5 January 2001, when the field is exited the value will be automatically updated with the leading zeroes to 2001-01-05.

Warning!

Changing Identifier 1 when multiple specimens are selected will result in all the selected specimens having the same primary identifier. This can make the specimens difficult to distinguish.

MEASUREMENT INFORMATION

The measurement information may also be edited like the specimen information. Click on the *Edit Metadata* icon to enable editing the measurement information. As you make your changes the data will be immediately updated for the selected specimens

Extremely Important Warning!

DO NOT CHANGE THE SPECTRUM TYPE UNLESS YOU ARE ABSOLUTELY CERTAIN IT IS NECESSARY!

Changing the specimen's type may cause unexpected side effects because it will change the interpretation of the spectral data. This may affect the colorimetric data, spectral graph scaling, simulated color and other items.

ENTERING NEW SPECIMENS

DATA EDITOR

When working with published data, new specimens may be created “from scratch” by clicking the “+” button below the Specimen List. This will cause the Data Editor to open. The window now has several additional fields to aid in entering the specimen. Here are the steps to make a new specimen.

Step 1. Select the type of specimen being created.

Step 2. Enter the starting wavelength. This must be greater than, or equal to, 200 nm.

Step 3. Enter the ending wavelength. This value must be less than, or equal to, 1100 nm.

Step 4. Enter the spectral sampling increment. SpectraShop can work with 1, 2, 4, 5 or 10 nm increments.

Step 5. Since some spectra have wide regions where the data values are the same, the Default Value is provided to fill all the spectral intervals with a common value. By default, this is set to 0.0 .


Step 6. The Value Range is provided to allow for 0-1 data values or for 0-100 values.

Step 7. Click on the Enter button to fill the data table with the values.

Step 8. Edit the value list with the desired values.

Step 9. Click Done to put the new specimen into the current collection.

Step 10. Edit the new specimen’s metadata to finish creating the specimen.

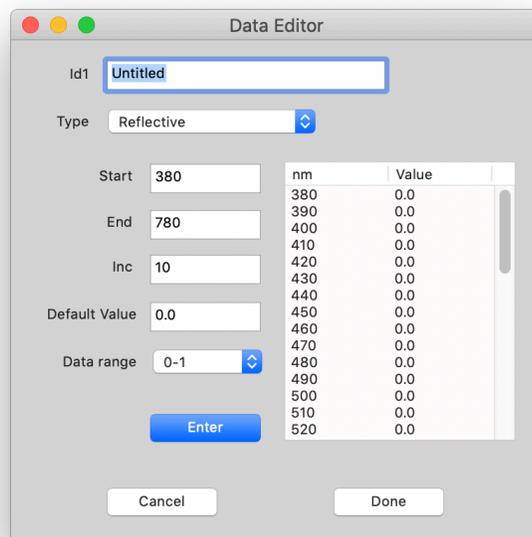

MEASURING

INSTRUMENT WINDOW

Spectral measurement begins by clicking either the *Measure Specimens* or *Measure Chart* buttons in the Tool window. For both of these choices, the first item to appear will be the *Instrument* window. In this window the measuring instrument, its options and hardware configurations are selected.

Depending upon the instrument and its options, after the connection is established, the window will show the options available for that instrument and the type of spectrum being measured.

Once the instrument and its operational options have been chosen, the appropriate specimen or chart measurement window will appear, depending on the selected *Specimen Type*.

After you have finished with the measurement, you may connect to a different instrument or change to a different specimen type. Changing from specimen to chart measurement, or vice versa, requires closing the *Instrument Connection* window, then clicking the desired *Measure Specimens* or *Measure Chart* icon.


Step 1. Choose an Instrument

Begin by selecting an instrument from the *Instrument* popup menu. If you pick an i1Pro it will connect automatically. For other instruments, click the *Connect* button to open communications with the instrument.

If the instrument connects with a serial interface, or, in the case of the PR-655/670, emulates a serial interface with a USB hardware connection, the serial port and possibly the baud rate must be set before clicking the *Connect* button.

As part of the connection process the serial number of the spectrometer is read from the instrument and displayed next to the *Connect* button. This verifies the connection has been made successfully.

Note: i1Pro instruments are automatically connected to SpectraShop.

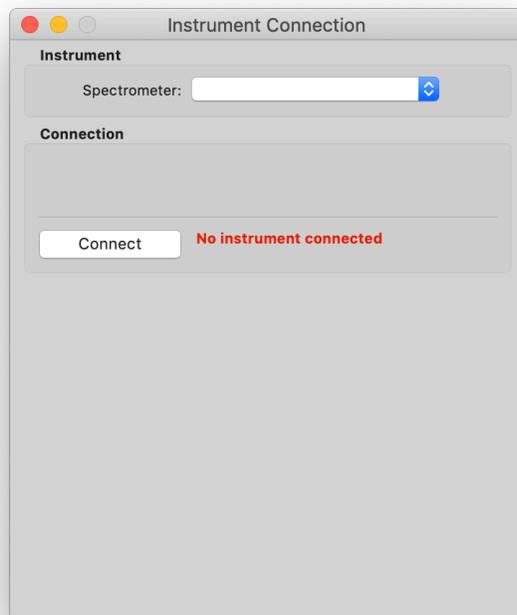

Step 2. Select Connection Options (Device Dependent)

The connection options appear only for some non-USB connected instruments.

Port

This option is only available for serial communication devices, e.g. Spectrolino, or ones that simulate serial devices, e.g. PR-655/PR-670. Select the port from the list presented in the popup menu.

Baud Rate

This option is only available for serial communication devices. Consult your device's manual and select the appropriate connection speed from the list presented in the popup menu.

Step 3. Connect to the Instrument

Click on the *Connect* button to open the communications with the instrument. Once the connection is established a verification message is displayed in green text next to the *Connect* button. If there is a problem initializing the connection, a message in red is displayed.

Step 4. Select Specimen Type

Spectrum Type

Depending on the instrument five types of spectra can be measured with SpectraShop:

- Emissive-flash (i1Pro1 and i1Pro2 only)
- Emissive-light
- Emissive-monitor
- Reflective
- Transmissive

The spectrum type and the choice of Specimen or Chart measurement will determine which window is presented for the actual spectral measurement.

Step 5. Select Instrument Options

Filter

Some instruments require adding or changing filters to the device for different spectral types. For example, the i1Pro requires an ambient diffusion filter be added for emissive-light measurements. Other spectrometers have filters to alter the way the spectrum is measured for various applications, such as a polarizer for glossy reflective measurements or a UV light blocking filter for reflective print measurements.

Most instruments measure emissive light sources with a diffusion filter attached. This serves two purposes; to diminish angular sensitivity of the device relative to the source and to minimize the chance of exceeding the instrument's range limit.

Geometry

The spectral type can also determine the instrument's measurement geometry. Some instruments have selectable geometries, such as integrating sphere instruments. After selecting the *Spectrum Type* and *Filter* the *Geometry* will either be automatically selected or the options available are presented in a popup menu.

Aperture

Instruments may have multiple apertures which can be switched programmatically or physically. The choice of an aperture can be very important, depending on the type of material being measured. For example, coarse woven cloth needs a larger aperture than a fine woven cloth.

Light Source

Some instruments offer user selectable light sources. The choice of light source often depends on the spectrum type and may require selecting a filter. Make sure the *Filter* and *Light Source* are in agreement. As an example, the i1Pro3 Plus requires putting an M3 Polarizer filter on the instrument when the M3 light source is chosen.

Step 6. Calibrate

After the connection is established and the instrument's options selected, follow the displayed calibration directions, then click *Calibrate*. It may take several seconds to calibrate the instrument. When the calibration is completed a message will be displayed confirming success.

Some instruments (e.g. ColorEye XTH) will require two calibrations; one for white, one for black.

Transmissive Calibration

Making transmission measurements with instruments that do not directly support it, such as the i1Pro, will require a measurement for the instrument and another for the light source. Instructions will be presented next to the *Calibrate* button to guide you through the process.

Once the instrument has been connected and calibrated, the specimen measurement window for the selected type will appear.

MEASURING SPECIMENS

COMMON MEASUREMENT INFORMATION

Specimen Information

The descriptive information for the measurements is entered into the *Specimen Information* area. When the measurement is complete this data will be attached to the spectrum and sent to the top-most collection window.

Each measurement window presents the information applicable to that specimen type.

Measurement Averaging

When taking measurements it is often necessary to take more than one measurement and average the results for the final result. SpectraShop allows for a maximum of 99 measurements per specimen. As each measurement is made a high pitched bell tone is sounded and a message is displayed to indicate the current measurement in the sampling sequence. When the final measurement in the series is taken a low pitched bell tone is sounded.

The measurement tone may be disabled for quieter operation by unchecking *Audio tone*.

When multiple measurements per specimen are being taken, fixing the spectrometer to a rigid fixture is recommended to minimize the variance between measurements. Many portable spectrometers have a photographic tripod attachment point for this purpose.

Start/Stop and Measure Buttons

Once the measurement parameters have been selected, click the *Start* button to begin taking measurements. The *Start* button initiates a timer that periodically checks the instrument, retrieving the spectral information if a measurement was taken by pressing the instrument's measure button.

The *Measure* button can be optionally used to take a measurement without pressing the instrument's measurement button. This is very useful for situations where pressing the instrument's button might move the instrument, affecting the result, or for situations where the instrument's button may be inaccessible.

Auto Naming

To aid with naming specimens, the *Auto Naming* feature can be activated by checking the *On* box. By default this is selected.

Auto naming consists of a root name, called *Preceding*, followed by a *Separator* character then ending with a numeric *Value*. The minimum number of digits for the numeric ending is selected from the *Digits* popup menu.

The *Separator* character may be chosen from the drop down menu, or a different character may be entered into the box.

MEASURE EMISSIVE-LIGHT SPECIMENS

Note: For emissive-light or emissive-flash measurements, most devices require an ambient filter, or a cosine-corrector, be added to the instrument.

Step 1: Set up the Auto Naming. (optional)

Step 2: Fill in the specimen information. (optional, but recommended)

This information is stored with each measured specimen. This is where the specimen documentation is entered. Since much of this information may be repeated for a series of specimens, it saves time over editing this metadata later.

Step 3: Set the measurement options. (optional)


Step 4: Select specimen routing. (optional)

Normally, as each specimen is measured it is added to the Specimen list in the current collection window. When measurements need to be analyzed with one of the tools, the specimens must be copied to the tool. This method usually is performed after the specimens are measured. It also takes extra time and effort for the copying operation.

Using the Specimen Routing feature makes it possible to analyze specimens as they are being measured.

To use this feature, check the box or boxes to select the tool window destination and use the drop down menus to choose the destination within the window (if multiple destinations are possible). For some specimen types the specimen may be routed to multiple analysis windows.

Step 5: Start measuring.

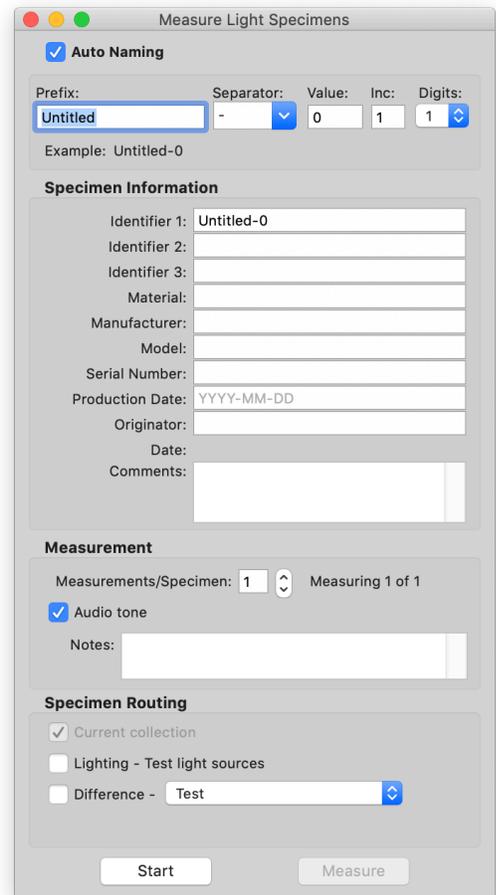

MEASURE EMISSIVE-FLASH SPECIMENS

Note: i1Pro Only.

Emissive-flash measurements are very similar to emissive-light measurements, with the exception that the instrument must be placed into a special mode to activate this feature. Currently, only the i1Pro and i1Pro2 instruments have this capability.

This mode operates just like the emissive-light mode, but there is a different way to operate the instrument's measurement button.

Begin this mode with the i1Pro by clicking the *Start* button. Then **press, and keep pressed**, the measurement button on the i1Pro. There will be a beep to let you know it is waiting for the flash, then fire the flash one or more times. **End the measurement by releasing** the measurement button. The flash specimen will be entered into the collection. One specimen is entered for each flash. In this mode the *Measurements/specimen* value is not used.

Note: Emissive-Flash measurements are only available with the i1Pro1 and i1Pro2 models. The i1Pro3 models do not support flash measurements at this time.

MEASURE EMISSIVE-MONITOR SPECIMENS

When the Measure Monitor Specimens window appears, a second Measure Monitor window also appears. The first one is the main window which controls the measurements, the second contains a single color patch. It is this patch that will be measured.


Note: the patch window may be resized to fit the requirements for the spectrometer or the desired sampling technique.

Auto Naming

There are two types of Auto Naming available for emissive-monitor specimens; the standard naming scheme, and RGB naming.

Standard Naming


The Standard Naming follows the same method used in the other measurement windows; a Preceding part, followed by an optional Separator, then ending with a numeric Value.

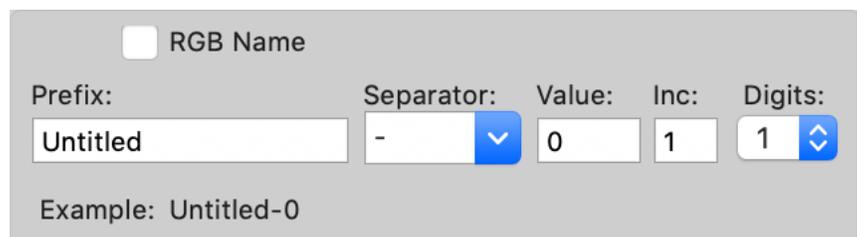

The screenshot shows a configuration panel for standard naming. At the top, there is an unchecked checkbox labeled "RGB Name". Below it, there are five input fields: "Prefix" with the text "Untitled", "Separator" with a dropdown menu showing "-", "Value" with the number "0", "Inc" with the number "1", and "Digits" with a spinner set to "1". Below these fields, the text "Example: Untitled-0" is displayed.

RGB Naming

It is possible to have the specimens named with the red, green and blue values used to specify the patch color. Check the RGB name box to switch to this type of specimen naming.

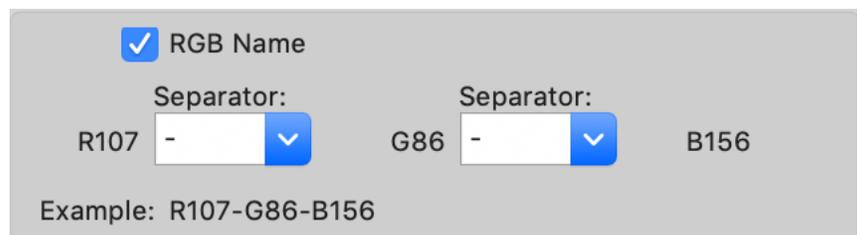

The screenshot shows a configuration panel for RGB naming. At the top, there is a checked checkbox labeled "RGB Name". Below it, there are three input fields: "R107" followed by a dropdown menu showing "-", "G86" followed by a dropdown menu showing "-", and "B156". Below these fields, the text "Example: R107-G86-B156" is displayed.

Measurement

Many spectrometers have a fixture for attaching the device to the monitor. Some of the fixtures use gravity to suspend the spectrometer from the monitor top with gravity holding the instrument against the display surface. Usually these fixtures have a method for blocking ambient light from influencing the measurement. Be certain the fixture lays flat against monitor's surface or the ambient light blocking will be compromised. Sometimes leaning the monitor backwards a few degrees will allow the spectrometer to lay flat.

If possible, turning out the room lights will reduce the opportunity for ambient light to get around the fixture's light blocking.

Another way to reduce ambient light is to cover the monitor and the attached spectrometer with a black cloth. Care must be taken with the cover that it does not affect the position of the instrument being flat to the monitor's surface. On LCD screens, be careful the dark cloth does not push the spectrometer's measuring aperture into the

screen surface. This can cause color shifts to occur at that pressure point and into some of the surrounding pixels, thus ruining the measurement.

There is another issue with measuring LCD monitors. These monitors work by shifting the polarization angle of the liquid crystals layered between two polarizers. Pixels are made to darken or lighten based on electronic control signals. However, the light emerging from the panel is polarized.

This is significant because most spectrometers based on diffraction gratings are sensitive to polarized light. The spectrometer will produce different intensity values depending on whether the LCD light is in alignment, or opposed to, the instruments polarization sensitivity direction.

To keep your readings consistent, do not change the rotation angle of the instrument in relation to the LCD screen's orientation. For more information on this subject, read the white paper [LCD Monitors and Spectrometers, an Interesting Problem](#).

RGB Patch

When the *Measure Monitor Specimens* window appears, another window is also shown that is filled with a color patch. This window should be placed so it is under the mounted spectrometer. The RGB values for this patch are set by entering values into the *Red*, *Green* and *Blue* fields, or by using the associated sliders. The range of values for each field is 0 to 255.

MEASURE REFLECTIVE SPECIMENS

Step 1: Set up the Auto Naming. (optional)

Step 2: Fill in the specimen information. (optional, but recommended)

Step 3: Set the measurement options. (optional)

Step 4: Select specimen routing. (optional)

Step 5: Start measuring.

Backing

When making measurements of reflective specimens, the choice of the material behind the specimen is very important. One of the optical properties of every specimen is its translucency. This is the amount of light that passes through the object. Translucency can range from totally transparent, passing all light, to totally opaque, not allowing any light through. Many specimens fall somewhere between these two extremes.

Since a spectrophotometer will measure any light arriving at its sensor, anything in the path of the illumination that affects the light will affect the measurement of the specimen's spectrum. This will include the specimen itself, any material on the back of the specimen and anything behind the specimen.

Objects on the back of the specimen will act as filters, modifying the transmitted light. This modified spectrum can be sensed by the spectrophotometer, depending on the material behind the specimen. One example of a back object would be any writing on the back of a paper; either a manufacturer's identification or notes written by someone.

The material the specimen rests on during the measurement is called the backing. The backing can have a very significant effect on a translucent specimen's measurement spectrum. A bright backing will reflect some light back through the specimen. The resulting measured spectrum will consist of the reflectance from the specimen, any material on the back of the specimen, the backing, and some of the specimen's transmitted spectrum.

A very dark backing will absorb the specimen's transmitted light, the effect of any material on the back of the specimen, and will not add any of its own spectrum to the measurement. It is for this reason that the ISO and ANSI specifications dictate a black backing with an optical density of 1.5.

The screenshot shows the 'Measure Reflective Specimens' software interface. The window title is 'Measure Reflective Specimens'. It features several sections: 'Auto Naming' with fields for Prefix (Untitled), Separator (-), Value (0), Inc (1), and Digits (1); 'Specimen Information' with fields for Identifier 1 (Untitled-0), Identifier 2, Identifier 3, Material, Manufacturer, Model, Serial Number, Production Date (YYYY-MM-DD), Originator, Date, Surface (Matte), and Comments; 'Measurement' with 'Measurements/Specimen' set to 1, 'Measuring 1 of 1', 'Backing' set to white, and 'Audio tone' checked; and 'Specimen Routing' with 'Current collection' checked and 'Difference' set to Test. At the bottom are 'Start' and 'Measure' buttons.

For some specimens the dark backing will make the measured spectrum different from the perceived one. An example is the spectrum of a mustard plant. When the flower petal is measured with a white backing the resulting spectrum matches with the perceived bright yellow color, with a tinge of greenness. A measurement with a black backing results in a spectrum with a strong green component. This is because the color of many objects in nature is a combination of the reflected light and the transmitted light. Also, only high lightness colors are perceived as yellow. When yellows are lower in lightness, they are perceived as browns and greens.

Thus, the choice of backing depends on several items. If the specimen is to be measured in accordance to a standard that requires it, then a black backing should be used. Any translucent specimen with writing on the back, or a different color on the back surface, such as electronic printer papers or paint store color brochures, should be measured with a black backing. A white backing should be used when a transmitted light component is a significant part of the specimen's perception. Examples of these specimens would be flowers and leaves, translucent papers with no writing or markings on the back and most fabrics.

Opaque objects are insensitive to the backing since no light is transmitted through the object to be effected by it.

When viewing printed samples, the backing for the samples must be the same as the measurement backing. Most printer papers are translucent, allowing the backing to influence the measurements. Using a different backing will result in the sample not matching the results predicted by the measurements. This is a common problem in viewing booths where the printer targets have been measured with a black or white backing but the final output sample is simply placed in the booth and viewed with the booth's gray as a backing. The output will appear too light (compared to a black measurement backing) or too dark (compared to a white measurement backing). Placing the same backing behind the output sample, then placing them together in the viewing booth will improve the evaluation.

SpectraShop offers several default values for the choice of backing; *white*, *black*, *self* and *n/a*. You may also enter your own custom backing value.

Reflective Measurements with the PR-655 or PR-670

When a reflective object is measured with the PR-655/PR-670 the result is a combination of the object's reflectance factors combined with the illumination. Other instruments with a fixed light source automatically remove the illumination component from the resulting spectrum to produce the reflectance factors only. To get this result with the PR-655/PR- 670 it is necessary to measure a standard white tile using the same illumination as for the reflective object measurement.

While many different white sources may work satisfactorily for a white reference, a sintered PTFE white tile is recommended. Available under the trade names of Fluorilon®, Spectralon®, and others, these tiles have a very high reflectance across the visible spectrum and they do not fluoresce. The white reference is measured during the calibration step when connecting to the instrument.

In addition to the calibration, the white tile's reference data (the certified reflectance factors that accompanied the tile from its manufacturer) must be entered into

SpectraShop. This is accomplished by opening the *Preferences* window, clicking on the *Miscellaneous* tab, then under the area *PR-655/670 Reflectance White Calibration*, click the *Open* button, then select the tile's reference file. This file is a SpectraShop binary file with **a single specimen**, the reference data.

MEASURE TRANSMISSIVE SPECIMENS

Step 1: Set up the Auto Naming. (optional)

Step 2: Fill in the specimen information. (optional, but recommended)

Step 3: Set the measurement options. (optional)

Step 4: Select specimen routing. (optional)

Step 5: Start measuring.

To measure transparent specimens with a device that does not have an inherent transparency capability, such as the i1Pro, some additional apparatus is necessary.

The basic requirements are a place to put the specimen on a constant full-spectrum light source. A light table can work very well for this purpose. Using a light table does present some challenges.

In spite of the best efforts from their manufacturers, light tables do not have a perfectly uniform illuminated surface. If a transmissive original, such as an IT8 4x5 transparency target was taped to the light table, the lighting change from one patch to another would introduce errors into the measurements. It is possible to overcome this problem by always measuring in the same place so the illumination is constant between measurements.

Begin by marking a spot on a light table where the measurements will be made. Make the marking slightly larger than the instrument's measuring nose so it will be visible as the instrument is positioned. This spot is measured during the calibration step in the Instrument window. It will be used as a reference for the subsequent transmissive measurements.

A light table surface is usually smooth, which may make it difficult to put the instrument into the same position between measurements. A template made from a thin piece of plastic can make the positioning much more consistent. Use either a colorless transparent or opaque black plastic to minimize the possibility of light reflected from the template affecting the measurements.

The most important item to consider in choosing a light table is the light source. It must be very constant in intensity and have a spectrum that extends beyond the range of the instrument (i.e. below 380 nm and above 730 nm for an i1Pro).

If the light source has low emission in part of the measured spectrum, then large errors will be introduced into the measured spectrum. One example of a good light source

Measure Transmissive Specimens

Auto Naming

Prefix: Separator: Value: Inc: Digits:

Example: Untitled-0

Specimen Information

Identifier 1:

Identifier 2:

Identifier 3:

Material:

Manufacturer:

Model:

Serial Number:

Production Date:

Originator:

Date:

Comments:

Measurement

Measurements/Specimen: Measuring 1 of 1

Audio tone

Notes:

Specimen Routing

Current collection

Difference -

would be a fluorescent lamp with a continuous spectrum, so there is no part of the spectrum with poor emission and it does not overheat the subject specimen.

There are also some new LED sources with full spectral emission. However, these are very new sources and may not be implemented in light tables, yet. The only way to be sure the light table will meet the required criteria is to measure the table. The areas to look at first are the violet region and the red region. First generation LEDs used a blue LED that excited a yellow phosphor to produce a white spectrum. Unfortunately, there is very little light emitted by these LEDs in the violet region below 420 nm and in the red region above 680 nm.

MEASURE CHARTS

MEASURE EMISSIVE-MONITOR CHARTS

Step 1: Open a chart file (required)

Begin by opening a predefined chart description file. The chart's name as defined in the file will appear next to the *Open* button. This chart file contains the list of all the patches with the patch Identifier and the associated R, G and B values.

Step 2: Enter monitor information (optional, but recommended)

The information unique to the monitor being measured should be entered before beginning patch measurement.

Step 3: Select measurement options (optional)

When taking measurements it is often necessary to take more than one measurement and average the results for the final result. SpectraShop allows for a maximum of 99 measurements per specimen. As each measurement is made a high pitched bell tone is sounded and a message is displayed to indicate the current measurement in the sampling sequence. When the final measurement in the series is taken a low pitched bell tone is sounded.


Once the measurement parameters have been selected, click the *Start* button to begin taking measurements. The *Start* button initiates a timer that periodically checks the instrument, retrieving the spectral information if a measurement was taken by pressing the instrument's measure button.

The *Measure* button can be optionally used to take a measurement without pressing the instrument's measurement button. This is very useful for situations where pressing the instrument's button might affect the result, for instance when measuring LCD panels where pressing on the display changes the screen's color.

Step 4: Start Measuring

Timing

With some monitors it is necessary to give the monitor some time to stabilize after changing the color patch display. A time delay of between 0.1 and 10 seconds, inclusive, can be selected from the *Time between patches* controls.

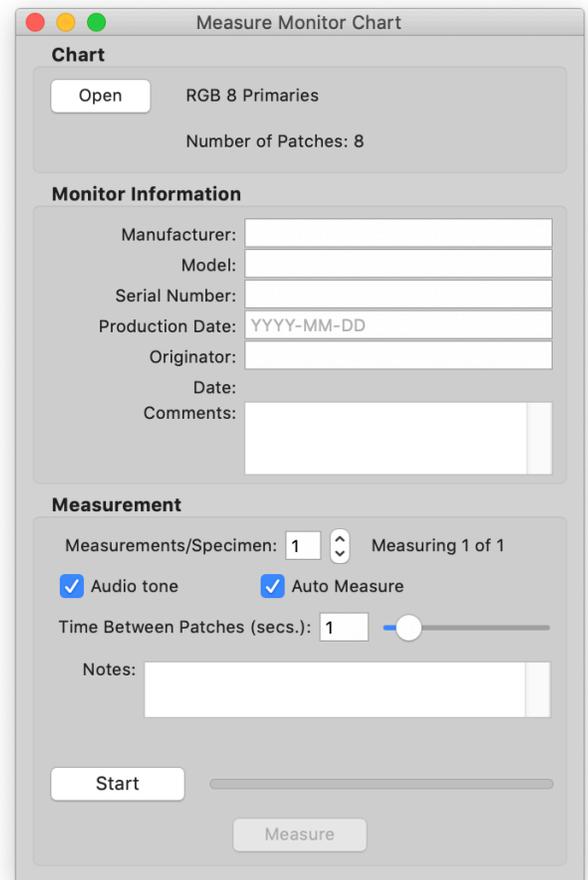


RGB Patch

When the *Start* button is clicked, a window appears that contains a color patch. This window should be placed so it is under the spectrometer. The RGB values for this patch are set by entering values into the *Red*, *Green* and *Blue* fields or by using the associated sliders. The values for each field must be in the range of 0 to 255.

MEASURE REFLECTIVE CHARTS

Step 1: Open a chart file (required)

Begin by opening a predefined chart description file. The chart's name as defined in the file will appear next to the *Open* button. This chart file contains the list of all the patches, their surface, and their locations in the chart.

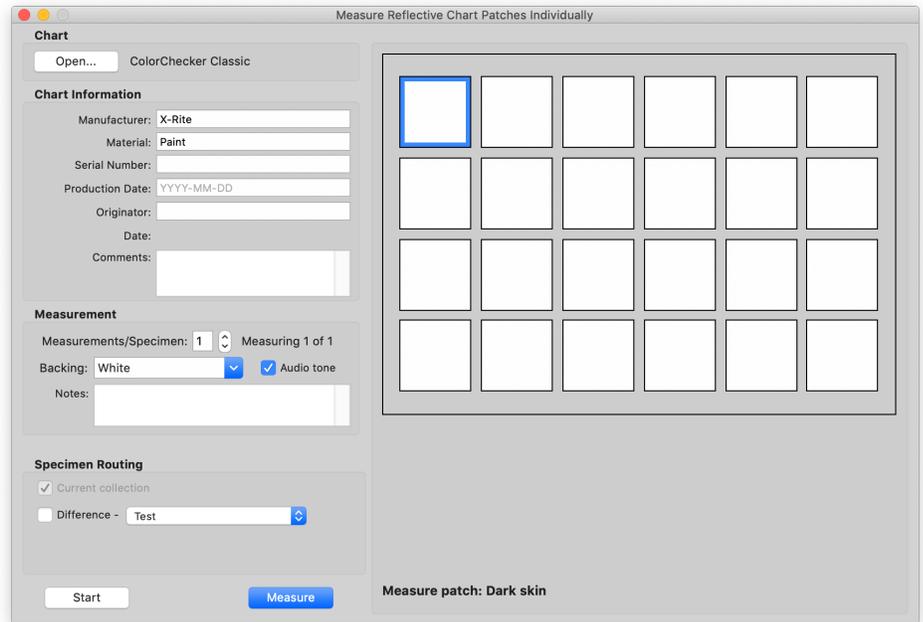

Step 2: Enter chart information (optional)

The information unique to the chart being measured should be entered before beginning patch measurement.

Step 3: Select measurement parameters (optional)

When taking measurements it is often necessary to take more than one measurement and average the results for the final result. SpectraShop allows for a maximum of 99 measurements per specimen. As each measurement is made a high pitched bell tone is sounded and a message is displayed to indicate the current measurement in the sampling sequence. When the final measurement in the series is taken a low pitched bell tone is sounded.

Step 4: Measure each patch

Once the measurement parameters have been selected, click the *Start* button to begin taking measurements. The *Start* button initiates a timer that periodically checks the instrument, retrieving the spectral information if a measurement was taken by pressing the instrument's measure button.

The *Measure* button can be optionally used to take a measurement without pressing the instrument's measurement button. This is very useful for situations where pressing the instrument's button might affect the result, for instance when measuring LCD panels where pressing on the display changes the screen's color.

Below the chart display a prompt is displayed prior to each patch's measurement. As each patch is measured it will be automatically entered into the current collection window. The chart display will update with the last measured patch's color.

When finished measuring the chart, close the window to end chart measurement.


MEASURE TRANSMISSIVE CHARTS

Step 1: Open a chart file (required)

Begin by opening a predefined chart description file. The chart's name as defined in the file will appear next to the *Open* button. The chart file contains the list of all the patches and their locations in the chart.

Step 2: Enter chart information (optional)

The information unique to the chart being measured should be entered before beginning to measure the patches.

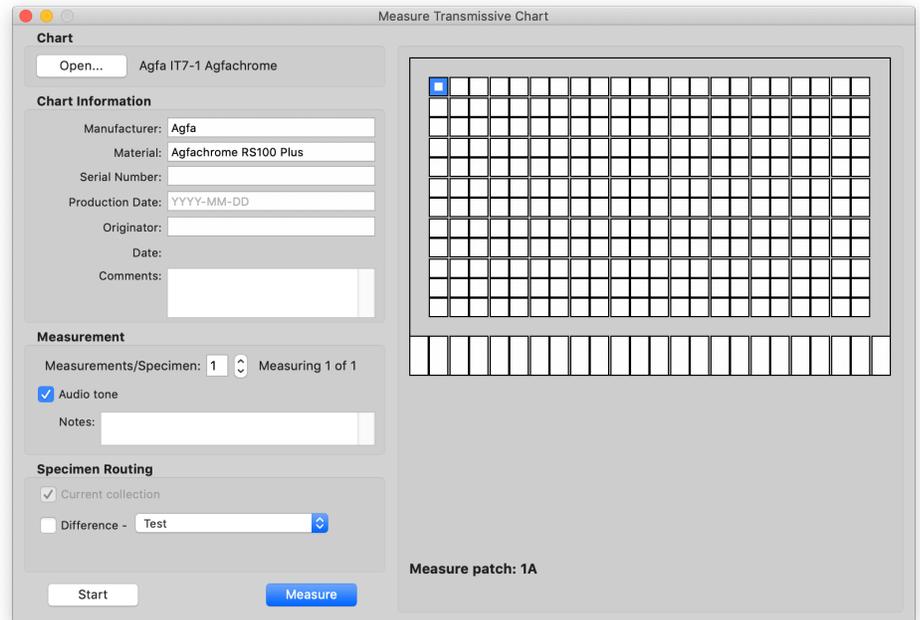

Step 3: Select measurement parameters (optional)

When taking measurements it is often necessary to take more than one measurement and average the results for the final result. SpectraShop allows for a maximum of 99 measurements per specimen. As each measurement is made a high pitched bell tone is sounded and a message is displayed to indicate the current measurement in the sampling sequence. When the final measurement in the series is taken a low pitched bell tone is sounded.

Step 4: Measure each patch

Once the measurement parameters have been selected, click the *Start* button to begin taking measurements. The *Start* button initiates a timer that periodically checks the instrument, retrieving the spectral information if a measurement was taken by pressing the instrument's measure button.

The *Measure* button can be optionally used to take a measurement without pressing the instrument's measurement button. This is very useful for situations where pressing the instrument's button might affect the result, for instance when measuring on a transparency viewer where the surface might deform with the weight of a hand.

Below the chart display a prompt is displayed prior to each patch's measurement. As each patch is measured it will be automatically entered into the current collection window. The chart display will update with the last measured patch's color.

When finished measuring the chart, close the window to end chart measurement.

CREATE A CHART


Clicking the *Define Chart* tool icon at the top of the collection window allows for the creation of chart definitions. The chart definition files are based upon the CGATS.17 standard with extensions and changes to support charts.

EMISSIVE-MONITOR CHART

Monitor charts consist of a series of RGB values to be displayed, then measured on a monitor.

Charts can be created in one of two ways; automatically and manually.

Automatically created charts

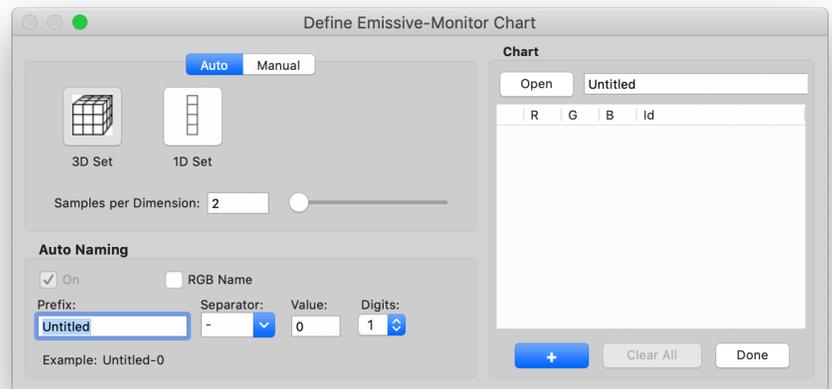

Charts can be created by varying the red, green and blue values to create a three-dimensional chart by selecting the *3D Chart* button. This type of chart is useful to determine the gamut of a monitor.

By selecting *1D Chart* a set of patches is generated with varying values for a single color selected from: red, green, blue, cyan, magenta, yellow or white. This type of chart is useful to measure the tonal reproduction curve for a monitor.

Once the parameters have been selected, clicking the + button will add patches to the chart patch list.

Note: Since patches are added, not replaced, when the + button is clicked, charts can be defined with a mix of 3D, 1D and manually generated patches.

Manually created charts

When manual patch definition is selected the red, green and blue values are individually defined by numeric entry in the appropriate fields or by using the sliders, then the + button is clicked to add the patch to the list.

Editing a chart

Patches can be removed from the chart patch list by clicking on the patch to remove then pressing the *Delete* key (Macintosh) or the *Backspace* key (Windows).

Multiple contiguous patches are selected by clicking on the first patch to remove then shift- clicking on the last patch to select the range.

Non-contiguous patches can be selected by using command-click(Macintosh) or control-click (Windows) to select each patch.

REFLECTIVE CHART


A reflective chart can be defined as a rectangular array of patches or as a set of arbitrarily positioned patches.

Rectangular charts are the most common type, represented by physical charts such as the X-Rite ColorChecker®.

An example of an arbitrary chart is the OECF chart in which the patches are arranged in a circular pattern.

Rectangular Chart

After filling in the physical description of the chart, corner descriptions and patch information, click the + button to add the patches to the patch list.

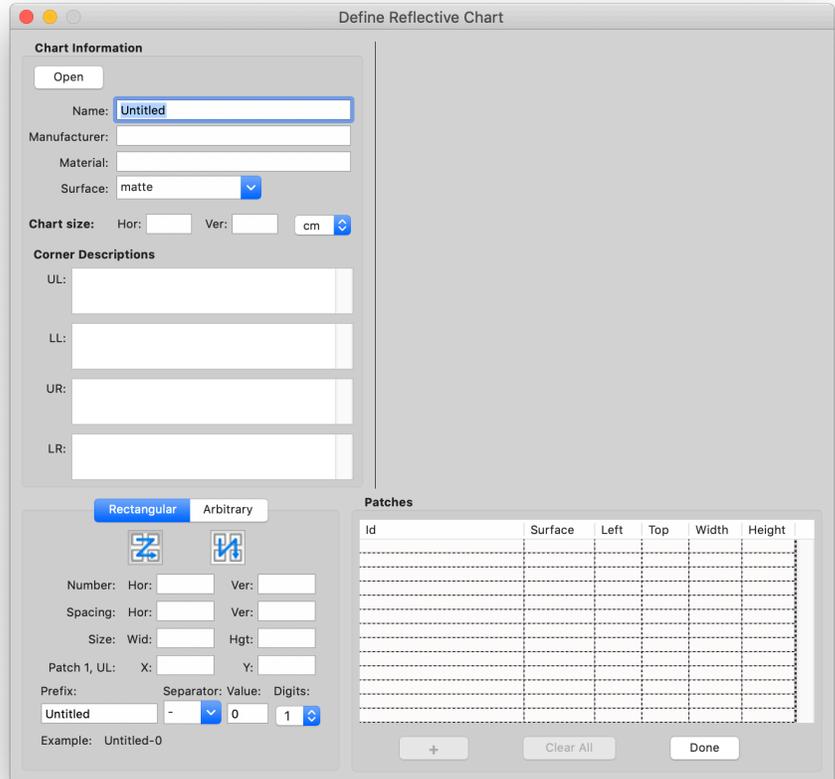

The *Corner Descriptions* are directions to an operator for locating the corner points of the chart. They are necessary because the physical corners of the chart are often not the ones used for locating patches. They allow the chart description file to be used for more than spectral measurements, such as processing images of the chart into XYZ or L*a*b* values.

After the patches have been entered into the list, the name and surface for each patch can be edited by clicking on the *Id* or *Surface* field in the patch list. The patch locations cannot be changed once they have been entered into the list.

However, it is possible to correct erroneous patches by deleting them then re-entering the patch. To delete one or more patches, click in the dimension area for the row with the patch to delete. The entire row will highlight. Press the *Delete* key to delete the patch from the list.

When the chart definition is complete, click the *Done* button. A dialog box will appear to allow for saving the chart definition or discarding it.

An existing chart definition can be edited by clicking the *Open* button and selecting the appropriate file. Then add or delete patches to make the new definition.

Arbitrary Chart

After filling in the definition for each patch, click the + button to add the patch to the patch list.

Since each patch can be added individually, any arbitrary layout of patches can be achieved.

TRANSMISSIVE CHART

A reflective chart can be defined as a rectangular array of patches or as a set of arbitrarily positioned patches.

Rectangular charts are the most common type, represented by physical charts such as the X-Rite ColorChecker®.

An example of an arbitrary chart is the OECF chart in which the patches are arranged in a circular pattern.

Rectangular Chart

After filling in the physical description of the chart, corner descriptions and patch information, click the + button to add the patches to the patch list.

The *Corner Descriptions* are directions to an operator for locating the corner points of the chart. They are necessary because the physical corners of the chart are often not the ones used for locating patches. They allow the chart description file to be used for more than spectral measurements, such as processing images of the chart into XYZ or L*a*b* values.

After the patches have been entered into the list, the name and surface for each patch can be edited by clicking on the *Id* or *Surface* field in the patch list. The patch locations cannot be changed once they have been entered into the list.

However, it is possible to correct erroneous patches by deleting them then re-entering the patch. To delete one or more patches, click in the dimension area for the row with the patch to delete. The entire row will highlight. Press the Delete key to delete the patch from the list.

When the chart definition is complete, click the *Done* button. A dialog box will appear to allow for saving the chart definition or discarding it.

An existing chart definition can be edited by clicking the *Open* button and selecting the appropriate file. Then add or delete patches to make the new definition.

Arbitrary Chart

After filling in the definition for each patch, click the + button to add the patch to the patch list.

Since each patch can be added individually, any arbitrary layout of patches can be achieved.

GRAPH TOOL

OVERVIEW

This tool creates two-dimensional graphs of any two colorimetric values. These graphs are created as groups of specimens, either singly or paired. These groups can be linked with lines or directional arrows.

GROUPS

Creating Groups

To create a graph, begin by selecting, then dragging, or copying and pasting, specimens to the group area of the 2D Graph Inspector from any open collection. A group will be created and the colorimetric values displayed in the Graph 2D window.

Each set of specimens dropped into the *Group* list creates a new group. Each group can be individually selected for display by checking or unchecking the box next to each group's name, as can each individual specimen within a group.

Renaming Groups

Each group can be renamed by selecting the group in the list, then entering a new name in the Name field.

Adding to a Group


When specimens are dropped into the *Specimen* list they are added to the currently selected group. Specimens are automatically displayed when added to a group. To hide a specimen, uncheck the *Show* box in the *Specimen* list.

SAVING A GRAPH

When the Graph2D window is frontmost, the graph can be saved to a file by using the *File/Save Graph* menu command. The file format can be selected from JPEG, PNG, GIF or TIFF in the *File Save* dialog window.

Note: All file types are not available on all platforms.

JPEG files are saved with the maximum quality setting to prevent any visible artifacts in the resulting image file.

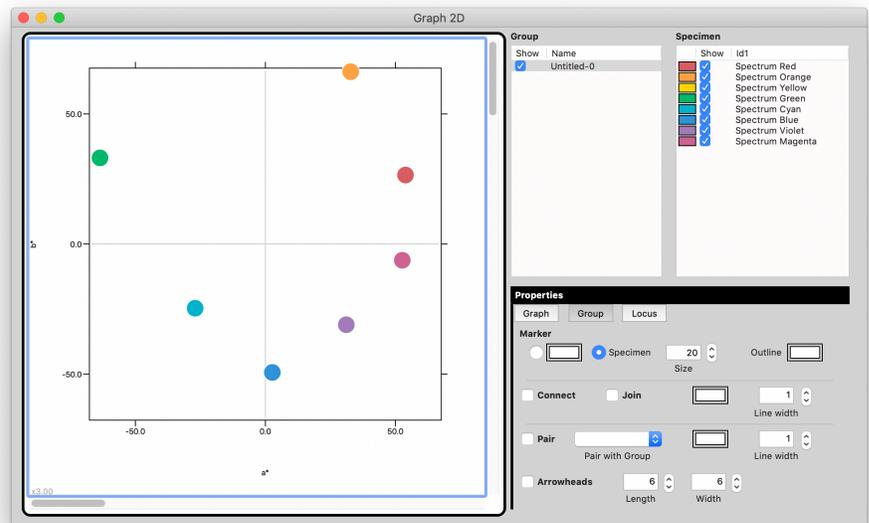

PRINTING A GRAPH

The graphs are created with sufficient resolution to allow for a minimum 10 inch print at a resolution of at least 300 ppi. To print the graph, select the *File/Print* menu command. Parameters relating to the printer's page definitions may be set using the *File/Page Setup* menu command. If the page has not been defined before the *Print* command is issued, *Page Setup* will be automatically executed before the *Print* command executes.

GRAPH 2D PROPERTIES

The properties are grouped by functionality represented by tabs at the top of the *Properties* area in the lower-right corner of the *Graph* window.

Graph Properties

Title

This is the title for the graph and it is displayed at the top of the graph window.

Axes

Any of the colorimetric properties may be selected for each graph axis.

When Specimen is selected for an axis, each specimen is listed along that axis versus the colorimetric value selected from the other popup menu. A maximum of 24 specimens can be displayed in this manner. One use for this feature is to display tonal reproduction curves.

Grid

Checking the box will display the grid with the grid lines in the selected color.

Background

This is the color used for the graph's background. The default is a white background with black spectral curve lines. This works well unless the specimen's color is to be used for the line and the specimen is very light. The background may then be changed to a darker one to improve the visibility of the spectral curves.

Line

These properties control the color of the line; an arbitrary color or the specimen's color, and the width of the line. The default is to use a black line, one monitor pixel in width.

Emissive Scaling

There are three choices provided for scaling emissive specimens.

Maximum of each scales each specimen so its maximum value corresponds to the 100% graph mark.

Maximum of all causes each specimen being graphed to be examined to find the one with the largest spectral maximum. All the other specimens are scaled to this value.

560 nm is often used to give all the displayed specimens a common reference point.

Group Properties

Marker

Each group may be drawn with its own marker size, outline color and fill color (or the specimen's color). This allows each group to be differentiated from other groups when more than one group is being graphed.



Marker control panel showing options for marker size and outline. The 'Specimen' radio button is selected. The 'Size' is set to 20. The 'Outline' is represented by a double-line rectangle icon.

Connect

All the members of a group can be connected with a line from member to member. This is a very useful property for showing gamuts and other group boundaries.




Connect control panel showing checkboxes for 'Connect' and 'Join'. A line width control is set to 1. The 'Join' checkbox is selected. A double-line rectangle icon is shown next to the line width control.

Checking the *Join* box will connect the last marker in the group to the first, creating a closed outline.

Pair

When the *Pair* box is checked individual members of a group will be connected by a line with the corresponding member of the group selected from the popup menu. If one group has more members than its pair, the number of pairings will be restricted to the group with the smallest membership.

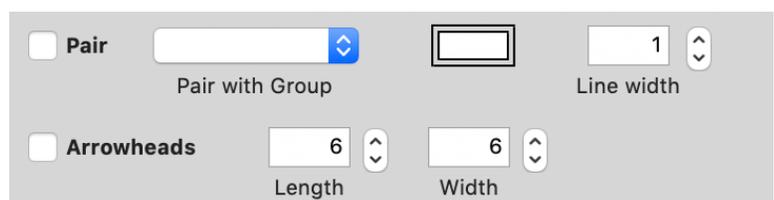

Pair control panel showing checkboxes for 'Pair' and 'Arrowheads'. The 'Pair' checkbox is selected. A dropdown menu is set to 'Pair with Group'. A line width control is set to 1. The 'Arrowheads' checkbox is selected. The 'Length' and 'Width' of the arrowheads are both set to 6.


Arrowheads

Checking the *Arrowheads* box will add arrowheads to each pairing line at the end of the line. The end of the line is always at the specimen in the group selected from the popup menu. One use for this feature is to show change trends between groups.

By carefully creating groups and pairings, spider graphs can be created.


Graph Examples

Tone Curve

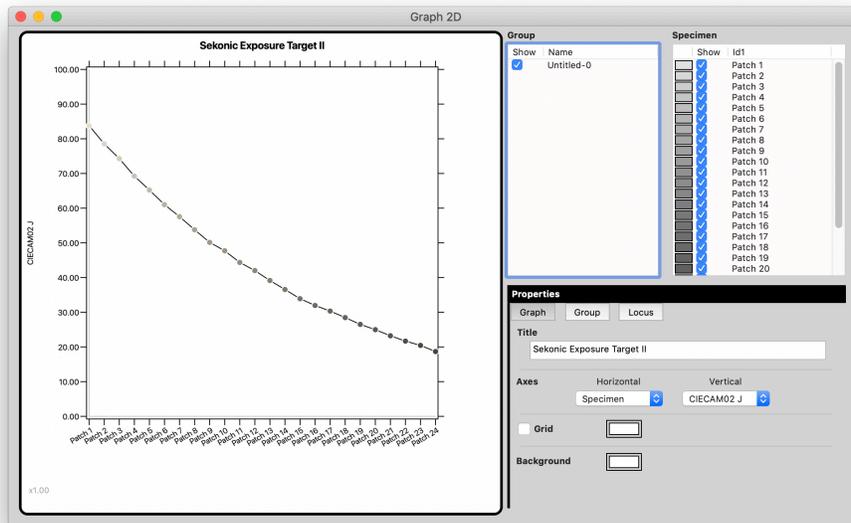


Graph of a single colorimetric value against the specimen's name.

Gamut Graph

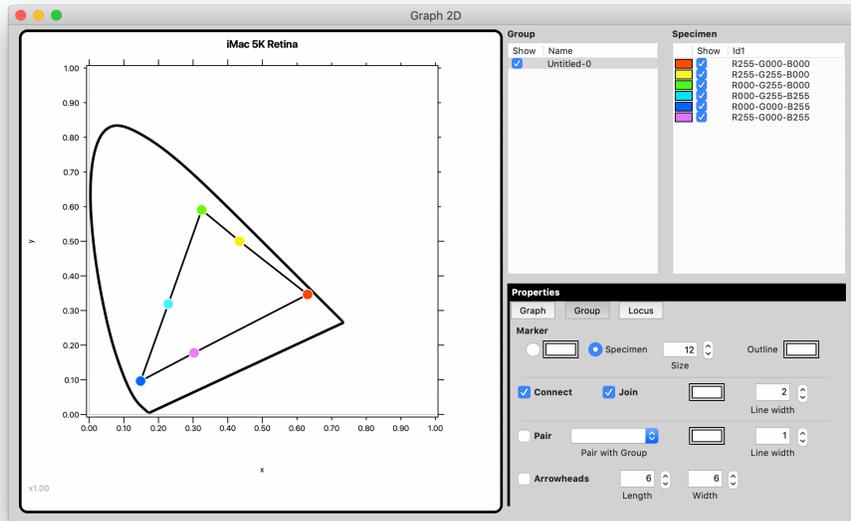


Classic xy gamut graph

Munsell 6/ Plane

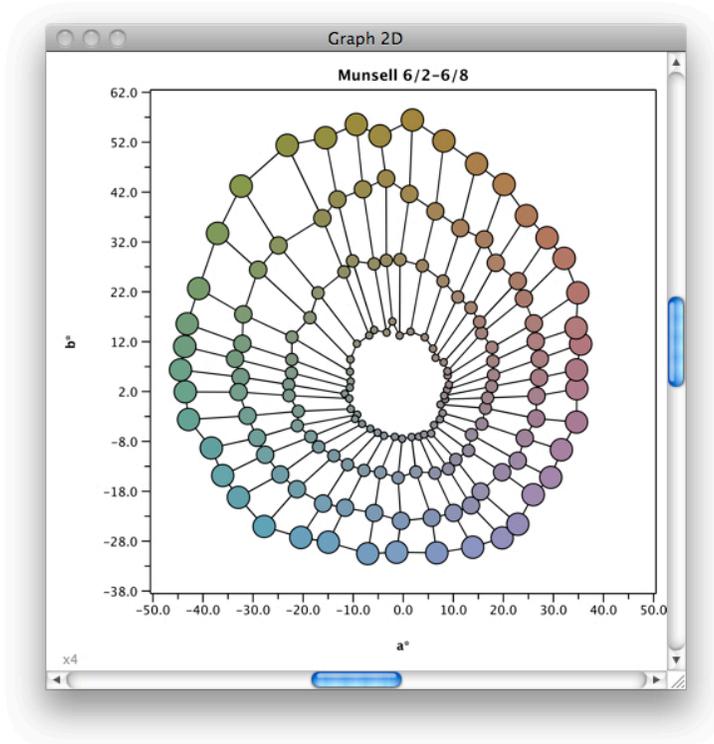

Spider graph showing the relationships of Munsell 6/ plane colors.

Print Reproduction Check

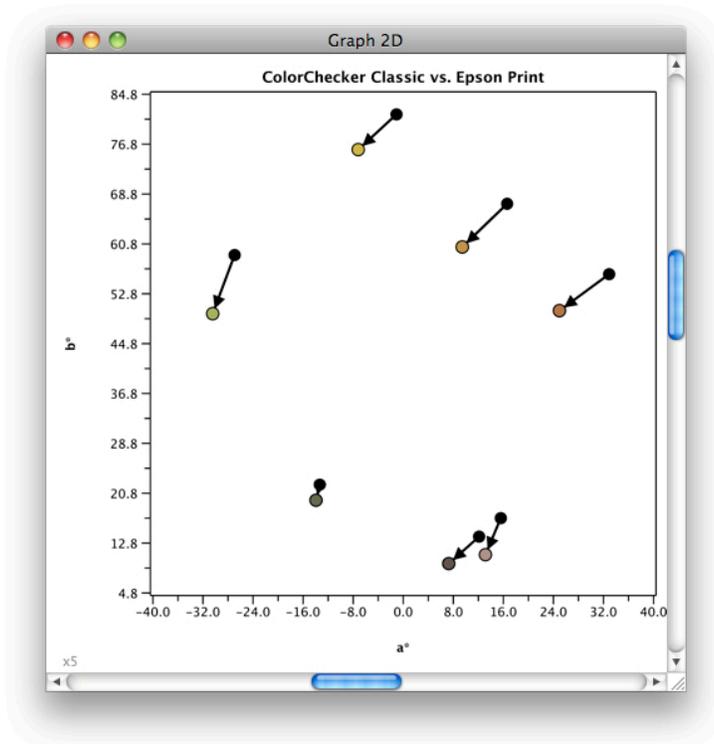

This example shows that some colors from a ColorChecker Classic (black dots) are reproduced on this Epson print (colored dots) with a cyan cast.

Locus Properties


The spectral locus will be displayed for xy and u^*v^* diagrams when the *Locus* box is checked. The line width and color for the locus are also selectable.

LIGHTING TOOL

When emissive-light specimens are dropped into the Test list the TM-30-18 and CRI metrics will automatically be calculated for each specimen. Highlighting a Test specimen will display its computed values.

CRI

The Color Rendering Index (CRI) is an old method intended to be a measure of how closely a light source mimics daylight. The standard CRI is calculated by simulating the test light reflected from 8 middle lightness, middle chroma colors and comparing the results with a simulation of a reference light source of the same correlated color temperature (CCT) as the test light source. For a CCT less than 4000 K, a Planckian, or blackbody, radiator is used for the reference. Above 4000 K a simulated daylight (i.e. D-series) reference source is used. The individual rendering indices (Ri) are averaged to obtain the General Color Rendering Index, reported as **CRI Ra**.

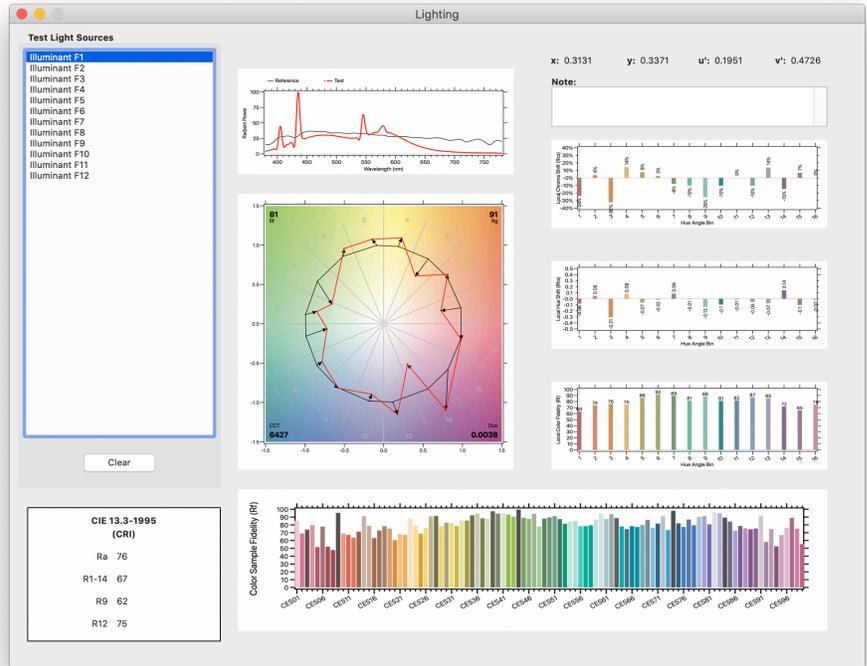

An additional 6 patches consisting of 4 high chroma patches, a flesh tone and a foliage patch are added to the 8 basic patches to create the Special Rendering Index, reported as **R1-14**.

In addition, the individual values for R9, a higher chroma red, and R12, a higher chroma blue, which are useful for some applications, are shown in the CRI box in the lower-left.

TM-30-18

This is the latest set of metrics intended to replace the older CRI system. Where CRI is based on 8 paint patches in the standard set, 14 paint patches in the full set, TM-30 is based on 99 patches representing printing inks, skin tones, plastics, fabrics, natural objects and paints. It is more representative of the wide range of materials with which light sources will be used.

TM-30 also uses a different scheme for creating the reference light source. For a CCT less than 4000 K, a Planckian radiator is used, above 5000 K a daylight reference is calculated, between 4000 K and 5000 K a blended light source

Spectral Graph

This graph shows the relative spectral power distribution for the test light source, shown in red, and the reference light source, shown in black.

Color Vector Graph (CVG)

This graph is the primary graphic for TM-30. It shows the gamut created by binning all the 99 individual samples and reference values into 16 bins based on their hue angle.

These 16 bins are shown as gray lines in the graphic, along with their bin numbers.

The reference gamut is shown as a black line, the test gamut in red. Arrows show the difference direction for each bin.

In the corners of this graphic are several important quality metrics.

Fidelity Index (R_f)

This is a specially scaled average of the differences between the 99 individual samples calculated for the reference illuminant and the test illuminant.

Gamut Index (R_g)

The R_g value is the ratio of the area spanned by the test bin coordinates in CAM02-UCS to the reference bin coordinates.

D_{uv}

The distance in the 1960 uv color space of the test light source from the reference light source line is displayed as D_{uv} . A negative value indicates the test source coordinates are more magenta/ red than the reference source. A positive value indicates the test source is more green/cyan than the reference source.

Sample Color Fidelity (R_{cs}) Graph

This graphic, located at the bottom of the window, shows the individual fidelity indices for all of the 99 samples.

Local Chroma Shift (R_{cs})

The radial shifts in the vectors of the Color Vector Graphic with each bar representing the chroma shift for each bin. This is a relative average chroma shift. For each of the 16 local chroma shift values, a negative value indicates a decrease in chroma, a positive value indicates an increase in chroma for the samples averaged within each hue bin.

Local Hue Shift (R_{hs})

The tangential shift in the vectors of the CVG for each bin are displayed in this graph. For each bin a negative value indicates a clockwise hue shift (e.g. orange toward red), a positive value indicates a counterclockwise hue shift (e.g. green toward blue).

Local Color Fidelity (Rf)

For each hue angle bin shown in the CVG, a hue specific measure of color fidelity is calculated and displayed here. The values range from 0 to 100, with higher values indicating better average similarity to the reference illuminant for the samples within each hue angle bin.


Note

A note may be added relating to the TM-30 analysis. It is not retained with the test specimen, existing only for inclusion on any report that may be generated.

TM-30 REPORTS

SpectraShop can create a *PDF report*, a file with the information contained in the Lighting window. To create the report, select *Create Report* from the *File* menu. The PDF file will contain a single page for each test specimen until pages for all the currently selected specimens have been created.


The report is formatted as suggested in the TM-30-18 standard.

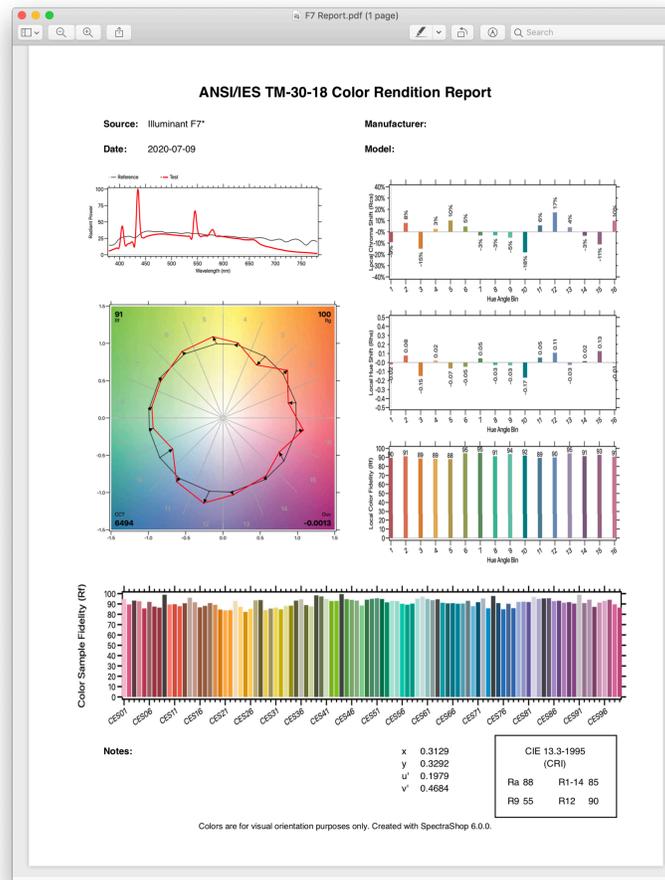

CALCULATOR TOOL

Spectral calculations may be performed with up to four sets of specimens with this tool.

After dragging and dropping a set of specimens from a Collection into the List 1 area, the numerical operation popup menu for List 1 will be activated.

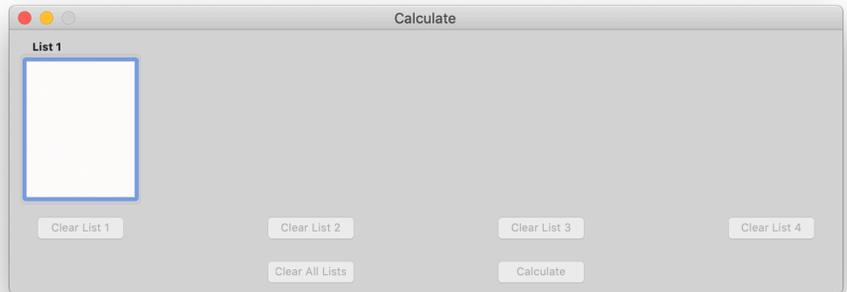

Depending on the selection from the first operation menu popup, List 2 list may or may not be activated. Operations that require only one operand (i.e. Average, Normalize, Scale by) will not enable the Spectrum 2 list.

Operators that require two operands (i.e. Add, Subtract, Multiply, Divide) will cause List 2 to be enabled for dragging and dropping the second set of specimens. Only two operand operators are permitted for the second and third operations.

Operations are performed by taking the first specimen in List 1, then performing the selected operation with the first specimen in List 2. The first List 1 specimen is then combined with the second List 2 specimen and so on until all the List 2 specimens have been combined with the first List 1 specimen. Operations continue with the second Spectrum 1 list specimen, and so on, until all the specimens of List 1 have been combined with all the List 2 specimens. If secondary or tertiary operations have been selected, the results from the first operation are combined with List 3 and List 4 specimens in a similar manner.

Note: This ability to cascade operations is a very powerful tool for performing some color analyses. For example; an illuminant could be placed in List 1, a reflective sample in List 2, with Multiply as the first operation, then a filter placed in List 3, with the Multiply operator for the second operation, and the spectral response of a sensor for List 4, again with the Multiply operator for the third operation. The result will then be a simulation of the sensor's spectral response for the reflective object in the color channel defined by the filter.

The results of these calculations are placed in the topmost Collection window. The identifier for the resulting spectra will be a combination of the original specimen identifiers and the operation performed. For example, "SpecimenA" added to "SpecimenB" will result in a spectrum with an identifier of "SpecimenA+SpecimenB".

Note: To allow any specimen, regardless of the sampling interval and range, to be combined with any other, all the calculations are performed with the 1 nm data used for the colorimetric calculations in each Collection window.

ADD

Each spectral band for each specimen in List 1 will be numerically added to the corresponding spectral band for each specimen in List 2. This is commonly used for combining colors in an additive situation, such as RGB color combining.

SUBTRACT

Each spectral band for each specimen in List 2 will be numerically subtracted from the corresponding spectral band for each specimen in List 1. One use for this function is to remove offsets from the specimens.

MULTIPLY

Each spectral band for each specimen in List 1 will be numerically multiplied with the corresponding spectral band for each specimen in List 2. This is a very commonly applied operation used to combine spectra for situations such as filters added to illuminants or light reflecting from an object's surface.

DIVIDE

Each spectral band for each specimen in List 1 will be numerically divided by the corresponding spectral band for each specimen in List 2. This operation can be used to ratio one spectrum to another such as when a spectrophotometer is calibrated to an arbitrary white reference and the white reference must be removed from samples measured with this setup to result in the measured sample's spectrum.

AVERAGE

The spectra of all the specimens in List 1 list are averaged together to result in a single spectrum. The statistics of the minimum, maximum and standard deviation for each spectral band are calculated for the averaged result.

NORMALIZE

Each specimen in the Spectrum 1 list is normalized to one of three choices; Maximum, 560 nm, or Wavelength.

Maximum will find the maximum response in each specimen's spectrum and normalize the spectrum to that value.

560 nm will cause the value for the 560 nm spectral band to be used to normalize the spectrum.

Wavelength will cause a field to appear adjacent to the Normalize Type popup menu. The spectrum will be normalized to the value corresponding to this wavelength.

SCALE BY

The spectrum will be multiplied by the value set in the numeric field below the operator popup menu.

DIFFERENCE TOOL


This tool allows for two types of comparisons; a list of specimens compared to a single reference specimen, or two paired lists of specimens.

Four combined metrics are computed; ΔE_{ab} , ΔE_{94} , ΔE_{CMC} and ΔE_{2000} . Any of these may be selected for the Pass/Fail indicator. Additionally, ΔCCT may be used for emissive-light specimens.

COMPARISON METHODS

Single Reference Comparison

Drag a specimen from any open collection into the Reference list. Then drag one or more specimens into the Test list. Each test specimen will be compared against the reference. A pass or fail indicator is displayed next to each test specimen.

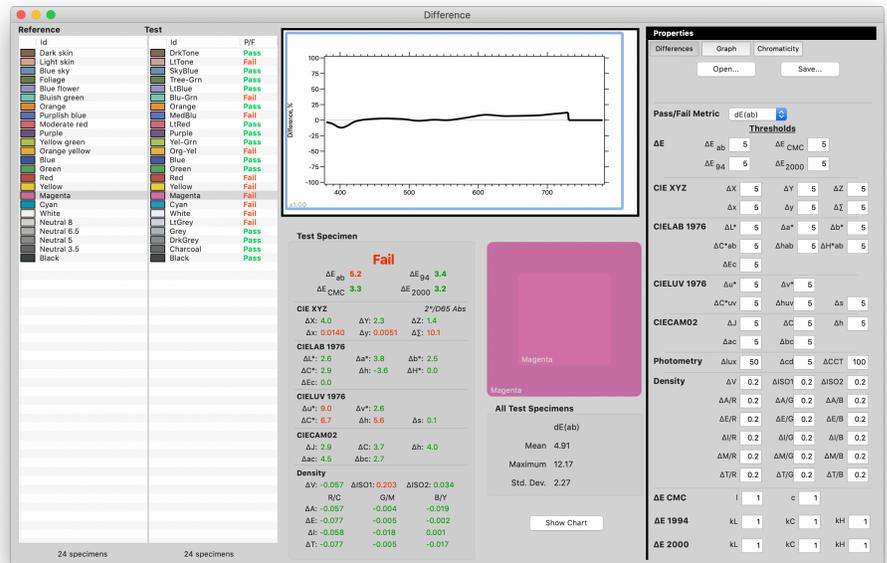

Selecting a test specimen will display all its calculated differences. For visual comparison, a simulated color patch is also displayed abutting a simulated reference color patch.

Paired Comparisons

When more than one specimen is placed in the Reference list, a paired comparison is created when specimens are dropped into the Test list. The comparisons are limited to the smallest list, additional specimens without a paired companion will not be used.

DIFFERENCE GRAPH

When a test specimen is highlighted, a graph is displayed showing the spectral difference at each wavelength. The graph uses 1 nm data so if any of the comparisons involve specimens with unequal ranges or specimens which do not extend across the entire spectrum then sudden transitions may occur at the ends of the measurement range.

Saving a Spectral Graph

The spectral difference graph can be saved to a file by using the *File/Save Graph* menu command. The file format can be selected from JPEG, PNG, GIF or TIFF in the File Save dialog window.

Note: All file types are not available on all platforms.

JPEG files are saved with the maximum quality setting to prevent any visible artifacts in the resulting image file.

Printing a Spectral Difference Graph

Difference graphs are created with sufficient resolution to allow for a minimum 10 inch print at a resolution of at least 300 ppi. To print the difference graph, select the *File/Print* menu command. Parameters relating to the printer's page definitions may be set using the *File/Page Setup* menu command. If the page has not been defined before the *Print* command is issued, *Page Setup* will be automatically executed before the *Print* command executes.

EXPORTING DIFFERENCE DATA

When the Reference and Test specimens have been specified, the difference data may be exported to a text file by selecting the *File/Export* menu command. A text file with a format similar to the SpectraShop text export is created which lists the ΔE values, the threshold values, the statistics for the entire test list and the Δ values selected from the *Data to Export* options.

DIFFERENCE PROPERTIES

Opening and Saving Difference Thresholds

The values defined in the *Weighting Factors*, *Pass/Fail Metric and Thresholds* fields can be saved to, or retrieved from, a file with the *Open* and *Save* buttons.

Weighting Factors

Some metrics require setting weighting factors used to enhance or diminish aspects of the resulting ΔE value. Weighting factors may be set for the ΔE CMC, ΔE 1994 and ΔE 2000 calculations.

Pass/Fail Metric

In addition to the individual tolerance thresholds, one of the following values may be selected to control a pass or fail indicator for the entire specimen:

ΔE_{ab}

ΔE_{94}

ΔE_{CMC}

ΔE_{2000} CCT

This indicator is useful when using the Difference tool for quality assurance and testing. It is displayed above the other difference values as either **Pass**, or **Fail**.

Thresholds

The Difference Inspector may be used to set the tolerance thresholds for all of the calculated metrics. These tolerances control the coloring of the values in the Difference window. Green text indicates the value is within the tolerance, red text for values outside their tolerance thresholds.

Difference Graph Properties

Grid

A grid can be displayed by checking the *Show* box. The color for the grid lines is selected by clicking in the *Color* box.

Background

The graph's background color can be selected by clicking in the associated *Color* box.

Line

Currently the difference graph is always displayed with a black line. However, the width of the line can be adjusted to improve the line's visibility.

Colorimetric Properties

Viewing Conditions

Here the *Observer* and *Illuminant* can be selected for the colorimetric calculations.

CIECAM02

The adapting field luminance is selected from the *Ambient Luminance* field and slider. The *Surround* popup menu selects the brightness of the area surrounding the specimen.

Graph Properties

Show Graph

Checking the *Chart* box will display the chart difference graph window. In this window a color coded chart can be displayed with each patch's color defined by the difference values. The values used are the ones currently specified as the *Pass/Fail* metric.

Difference Zones

The zone boundary difference values are specified in the *Delta values* numeric fields below the zone patches. The number of zones and their colors are fixed to five with the given colors.

Chart

The chart displayed in the difference chart window can be either a reflective or transmissive chart which has been defined with the *Define Chart Tool*. It is selected with the *Open* button and its name will be displayed next to the button.

The color to use for the chart's background is selected with the *Surround* color box.


SPECTRAL SEARCH TOOL

This tool searches through the currently open collections for spectral matches to the specified list of specimens.

Search Within

When the Search Tool is opened, all the currently open collections are listed here.

The checkboxes next to each collection's name may be used to control which collections are to be searched for matches to the specimens.

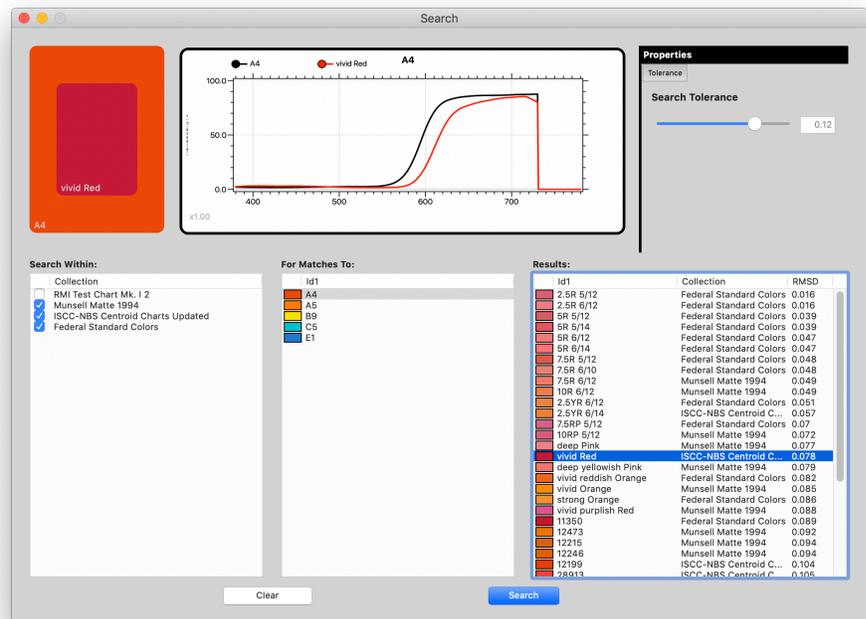

For Matches To

This is where the specimens to be matched are placed, either by drag and drop or by Copy/Paste.

Search Results

Once all the specimens to match are placed in the *For Matches To* list, click the Search button to start the matching process.

As each specimen in the *For Matches To* list is selected, a list of matching specimens is displayed in the *Search Results* list. Highlight each result to see a graph of the original specimen and the currently selected match.

The matches are created by calculating the Root Mean Square Difference (RMSD) between the original specimen's spectrum and each spectrum in each search collection. Any specimen who's spectrum is less than the *Search Threshold* value specified in the Tolerance section of the Properties, is added to a list for each original specimen.

SPECTRAL SEARCH PROPERTIES

Only one property is available for this tool, the Search Tolerance. This value controls the threshold for when a test specimen is considered a match.

CREATE LIGHT SOURCE TOOL

This tool creates light source specimens, either Planckian or D-Series.

Type



Select the type of light source to generate.

Planckian

These sources are also called blackbody radiators because these sources would emit energy perfectly and would also absorb light perfectly, such as an ideal black object.


The physicist Max Planck developed an equation which predicted the form of the spectral power distribution curve for different temperatures, so this type of radiator was named after him.

Planckian radiators are usually specified for light sources with correlated color temperatures less than 4000 K, although Planck's equation can be used for higher temperatures. An example of a Planckian radiator is a tungsten filament bulb.

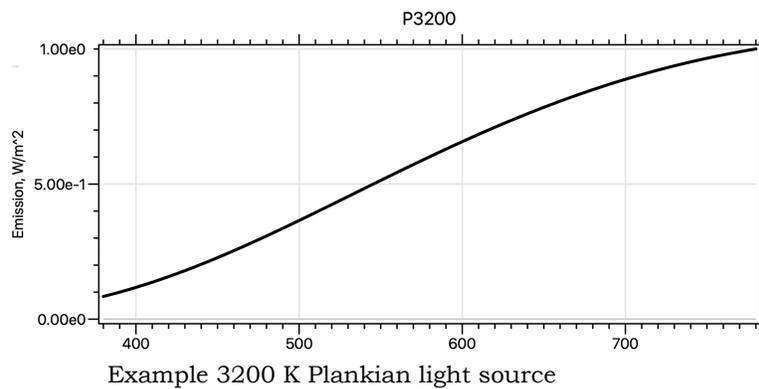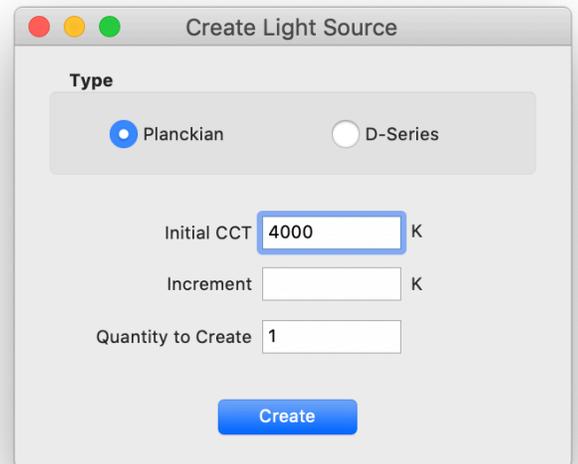

D-Series

The D-series spectra represent natural daylight. The equations used for computing a D light source are valid from 4000 K to 25,000 K.

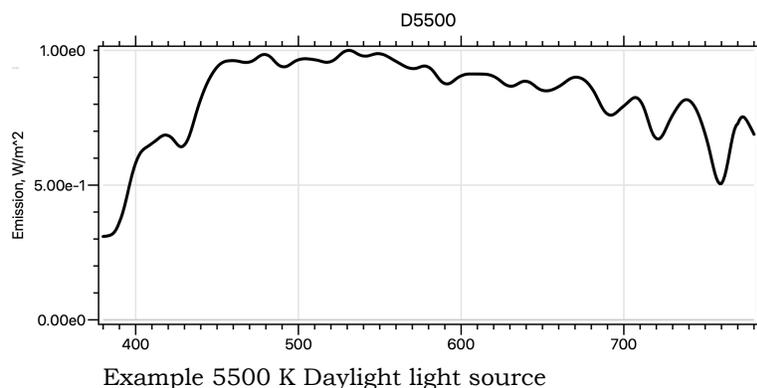

Initial CCT

Both the Planckian and D-series illuminant equations are specified by the Correlated Color Temperature (CCT).

Increment

When creating multiple specimens, this specifies the CCT increment between specimens. For single specimen creation, the Increment is ignored.

Quantity to Create

More than one specimen may be created by setting this value greater than one.

For example, a series of 5 light source specimens may be made in 100 K increments by setting the *Increment* to 100 and the *Quantity to create* to 5.

IMPORT

SpectraShop can import spectral data in several different file formats. Some formats are for importing specimens from other programs, some formats are the only way SpectraShop can get data from some instruments. The Import facility can also import the data stored on a PR-655/670 instrument's memory card.

SUPPORTED FORMATS

- CGATS 17, an ANSI standard color interchange format.
- CGATS, the X-Rite version.
- ColorMunki.
- MeasureTool, a program from the former GretagMacbeth, now X-Rite.
- SOCS spectral data.
- SpectraShop 1, 2, 3 and 5.
- Spectro 1, Spectro 1 Pro.
- Spreadsheet data, horizontal format.
- StellarNet.
- Photo Research PR-655/PR-670 internally stored data.

CGATS 17

This is an ANSI standard format for interchanging colorimetric, density and spectral information between programs. There are ASCII and XML versions of this standard. At this time, only the ASCII version is supported by SpectraShop.

Note: Only reflective and transmissive measurements are supported by the CGATS.17 standard.

Note: SpectraShop will import only the spectral data from CGATS.17 files. Colorimetric files will not be imported and for files with both colorimetric and spectral data, only the spectral data will be imported.

ColorMunki

The ColorMunki is an X-Rite Instrument. This file format is exported from the X-Rite ColorMunki application.

MeasureTool

This is a program for capturing measurements from a variety of X-Rite and GretagMacbeth instruments. Only reflective measurements are exported from MeasureTool.

SOCS

This format is defined in ISO/TR 16066:2003, Graphic technology—Standard object colour spectra database for colour reproduction evaluation (SOCS).

SpectraShop 1, 2, 3, 5

This format is based on the CGATS.17 format, but extended to include the additional metadata processed by SpectraShop but not found in CGATS.17. All the supported spectral types can be imported.

Note: the import file must include spectral data. Colorimetric only files will not be imported.

Spectro 1, Spectro 1 Pro

The Spectro 1 and Spectro 1 Pro are new instruments from Variable. They connect by Bluetooth to iOS devices. This format is exported from the iOS application supplied with the Spectro 1 or Spectro 1 Pro.

Spreadsheet Data, Horizontal

This is a spreadsheet file with comma separated values. Only spectral data is supported in this format. The data is stored as one line of header information, then each subsequent line is one specimen.

StellarNet

The SpectraWiz program used with StellarNet spectrometers exports this format.

PR-655/PR-670

The PR-655 and PR-670 are non-contact telespectroradiometers. They can store data either in their internal memory or on an SD memory card. SpectraShop can import the data from the SD card, not from internal memory. There are some restrictions on how the data is stored.

The PR-655/PR-670 stores multiple spectra into each data file on the card. Since the PR-655 can measure emissive, reflective and transmissive objects in any order, the spectra stored in each file could be a mixed collection of types. **SpectraShop requires that each file contain only a single type of specimen.** For example, all the spectra in a single file might be from reflective specimens. If multiple spectral types are to be measured, be sure to separate them into different storage files.

The second requirement is that **for reflective and transmissive files, the first spectrum in each file must be the white calibration tile.** SpectraShop will use this white tile data to properly scale the remaining spectra in the file. In the same manner as

direct connect measurements, if a reference file has been opened in the Preferences for reflective specimens, the spectra will be imported as *absolute* referenced. Reflective specimens imported without the reference file will be marked as *relative*.

Here are the steps to import the PR-655 or PR-670 files.

1. Be sure the PR-655 or PR-670 is plugged into a USB port prior to selecting the *File/Import/PR-655* menu command.
2. Select the *File/Import/PR-655/PR-670* menu command.
3. Select the USB port into which the PR-655 or PR-670 is connected.
4. Click the *Connect* button. SpectraShop will attempt to open a connection to the PR-655/ PR-670.
5. If the PR-655 or PR-670 was not connected, click *Connect* a second time.
6. If the connection is not made then cancel the import process, reset the PR-655 or PR-670 then start the import process again.
7. If it is successful the PR-655 or PR-670 serial number will be displayed in green text, then the instrument's file directory will be listed.
8. Select the files to import by clicking on the directory entries. Multiple entries may be selected by using the shift-click for contiguous files or the command-click (control-click on Windows) for non-contiguous files.

One or more files must be selected before the *Import* button is enabled. 9. Click the *Import* button.

10. Each file will be imported into its own new collection with each contained spectrum entered as a separate specimen.

a. If a CR-655 or CR-670 cosine corrector is used for the measurements then the specimen types will be entered as emissive-light.

b. If the MS-75 lens is used for the measurements then a window will appear to allow for selecting the specimen type. This will appear only once at the beginning of the import process for the instrument's file. Remember, all the specimens in a file are assumed to be of the same type. **Reflective and transmissive files MUST have a white calibration as the FIRST measurement in the file.**

11. Edit the collection to add the appropriate specimen information, then save the collection.

12. When finished importing files, click the *Disconnect* button or close the window to return the PR-655 or PR-670 to normal operation.

EXPORT

SpectraShop can export spectral data in several different file formats for working with the data in other programs.

SUPPORTED FORMATS

SpectraShop 3

This file format is based on CGATS.17, but extended to handle all the spectral types and metadata used by SpectraShop. All the colorimetric values can be exported.

MeasureTool

This is a program for capturing measurements from a variety of X-Rite and GretagMachbeth instruments. Only reflective measurements are exported from SpectraShop.

CGATS 17

This is an ANSI standard format for interchanging colorimetric, density and spectral information between programs. There are ASCII and XML versions of this standard. At this time, only the ASCII version is supported by SpectraShop.

Note: Only reflective and transmissive measurements are supported by the CGATS.17 format.

The CGATS.17 format supports several types of colorimetric values which can be selected from the *Data to Export* section. Spectral data and colorimetric data can be exported in the same file. Along with the colorimetric data, the observer and illuminant will be included in the file's metadata.

Raw Spectra

There are a few programs that need raw spectral data only, usually for a single specimen. This format allows multiple spectra to be exported, but no metadata is included in the file. Wavelength and response are the only information. Multiple specimens are separated by a blank line.

Note: Because there is no metadata, not even an identifier, exporting with this format is very risky and should be used only if you have a program needing such basic data.

InCamera Illuminant

The camera profiling application InCamera uses a version of the SpectraShop 2 export format for its custom illuminant files. This file will contain a single emissive-light specimen with a minimum of metadata.

Data Reference

Used to select the reference for the data; absolute or relative. Absolute referred data is referred to an absolute physical standard, such as W/m^2sr . Relative data is referred to a particular spectrum, such as referencing monitor colors to the monitor's white spectrum.

Data Format

The CGATS.17 format allows for spectral data to be expressed in the range of 0.0 to 1.0, or in the range of 0.0 to 100.0%. The upper values represent the normal data limit, they are not absolute limits; data is not compressed or clipped to fit within these ranges. Fluorescent objects are an example of reflective objects that often exceed 100% reflectance.

PREFERENCES

Note 1: Preferences are applied to the appropriate window when that window is opened, they are not applied to already open windows.

Note 2: To temporarily change preferences to an already open window, use the window's preference controls located within the window.

COLLECTION PREFERENCES

Spectral Graph

Vertical Axis

Use this setting to choose linear (default) or logarithmic scaling for the vertical axis.

Logarithmic scaling is very useful with dark specimens.

Emissive Scaling


Graphing emissive light spectra can present a problem for setting the scale. There can be a wide variance in the luminous flux from different sources which makes meaningful graphic comparisons problematic. SpectraShop presents a choice between *560 nm*, *Maximum of each* or *Maximum of all* value scaling.

When white light sources with relatively smooth spectra are displayed it is often the practice to scale the graph data so each spectrum has its 560 nm value at 1 on the graph's scale.

This may create a visual problem for sources that have 560 nm data with very low or high values in relation to the other spectra being displayed. It also does not work for non-white light sources, such as a red LED with no appreciable value at 560 nm.

When comparing monochromatic or non-white sources the *Maximum of each* option will find each specimen's maximum spectral value, using it to scale the graph to place this value at 1 on the scale. This may make darker specimens appear to be as bright as much brighter specimens, but it can make it easier to compare spectral features.

A better choice for comparing the relative magnitude of the light sources is the *Maximum of all* option. All the selected specimens are examined to find the overall maximum value, then this value is used to scale all the specimens.

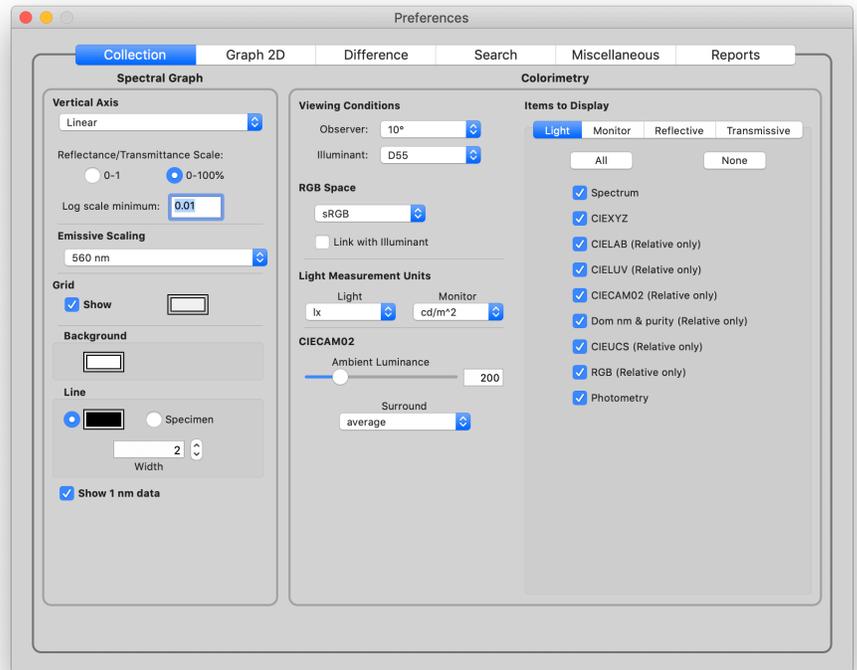

Grid

A grid can be displayed by checking the *Show* box. The color for the grid lines is selected by clicking in the *Color* box.

Background

The graph's background color can be selected by clicking in the associated *Color* box. This is a useful feature for improving the visibility of spectral graphs when the specimen's color is used for the line and the background color is similar to the specimen's color.

Line

This section controls the display of the specimen's line graph. The line color can be chosen to be the one in the *Color* box or the color calculated from the specimen's spectrum. When the *Specimen* color is used it is sometimes necessary to change the background color to improve the line's visibility.

Show 1 nm data

All spectra that are not natively sampled at 1 nm intervals are interpolated by SpectraShop internally to 1 nm. The resulting 1 nm spectrum can be displayed by checking *Show 1 nm data* from the *Spectral Graph Properties* section.

Colorimetry

Viewing Conditions

You may specify the default observer and illuminant for new collections by selecting values from the popup menus.

RGB Space

This is used for the conversion of XYZ coordinates into RGB values. When SpectraShop is opened for the first time sRGB is the default RGB space.

The *Link with Illuminant* checkbox is very important. When this is checked, the list of available RGB spaces for selection is limited to those RGB spaces with the same illuminant as specified in the *Viewing Conditions*.

As an example, when the *Viewing Illuminant* is set to D65 and the *Link with Illuminant* box is checked, only *Adobe 1998*, *Apple*, *HDTV*, *SMPTE-C* and *sRGB* spaces may be selected. When D50 is the *Viewing Illuminant*, only *Beta*, *Colormatch*, *eciRGB V2*, *ProPhoto*, *ProStar* and *Wide Gamut* RGB spaces are available for selection.

Unchecking *Link with Illuminant* should only be used by advanced users who have special needs for doing this.

Light Measurement Units

The amount of light flux illuminating a point is reported in lux or in W/m^2 , depending on the Properties setting.

For monitors, the light emitted from a point on the display's surface is expressed as cd/m^2 , or $W/(m^2 \cdot sr)$, depending on the Properties setting.

The light measurement units for emissive specimens can be selected from the appropriate popup menus.

Light: illuminance (lx) or irradiance (W/m^2)

This is the amount of light impinging on a place from the light source.

Monitor: luminance (cd/m^2) or radiance ($W/(m^2 \text{ sr})$)

This is the amount of light exiting the surface of the display.

CIECAM02

The adapting field luminance is selected from the *La* field and slider. The *Surround* popup menu selects the brightness of the area surrounding the specimen.

Items to Display

Use the tabs to switch between the different spectral types; *Light*, *Monitor*, *Reflective* or *Transmissive*. Then choose which colorimetric values will be displayed in the collection colorimetry area for each of these spectral types.

GRAPH 2D PREFERENCES

Graph

Axes

Select the default colorimetric values when the Graph Tool is opened.

Set the graph defaults to show a grid, in a particular color, and the color for the axes.

Background

This selects the default background color for the graph.

Marker

Here the choice of default color for the data markers can be chosen between a specific color for all the markers, or each data points individual color.

In addition, the size of each marker, in points, and the outline color for each marker may be selected.

Connect selects automatically connecting the markers in a graph group. *Join* selects adding one more line to connect the first and last markers in the group.


The connection line's color and size may also be set here.

Pair Line

When groups are paired, the default pair line color and size are selected here.

Spectral Locus

By default, the spectral locus may be shown in each graph. The choice of locus is selected from the popup menu. The color and line width for the locus may also be set here.

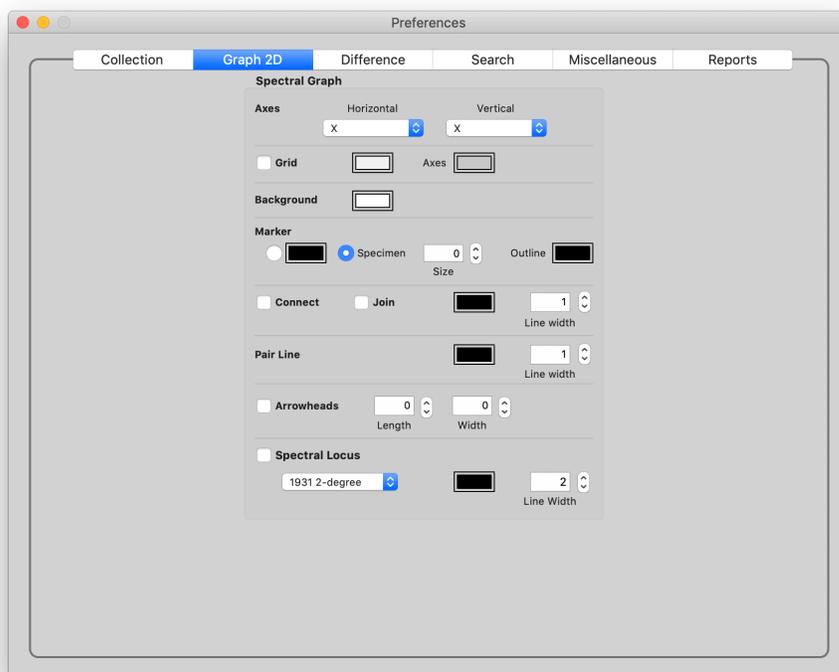

DIFFERENCE PREFERENCES

Spectral Graph

Grid


Set the difference graph to always show a grid by default.

Background

This selects the default background color for the difference graph.

Line

This sets the color and line width to use for drawing the difference graph spectrum.

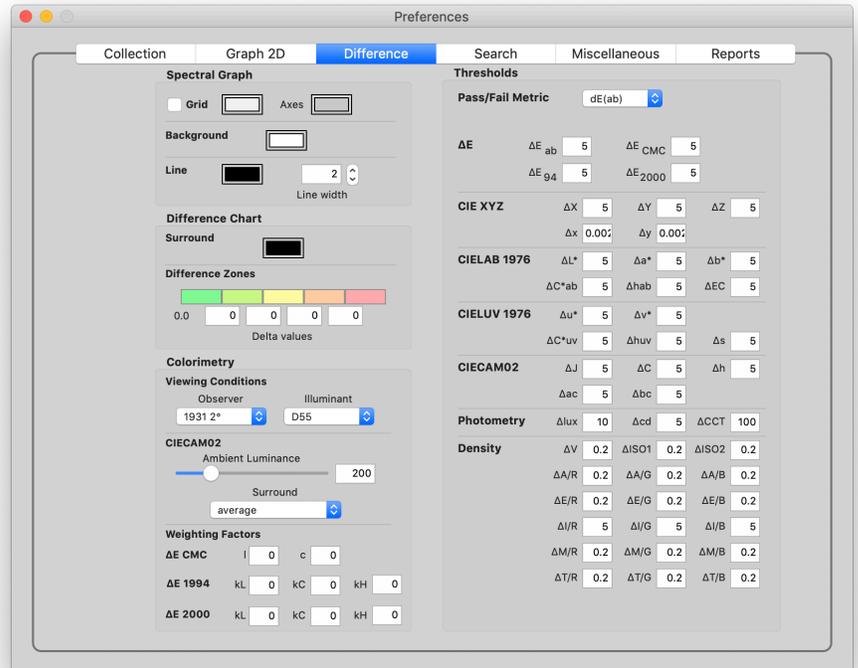

Difference Chart

Surround

When drawing a difference chart, this sets the default color for the space between each patch.

Difference Zones

Each patch in the Difference Chart is assigned a color depending on the ΔE value for that patch. The thresholds for each ΔE are set here.

Colorimetry

Viewing Conditions

You may specify the default observer and illuminant for new collections by selecting values from the popup menus.

CIECAM02

The adapting field luminance is selected from the L_a field and slider. The *Surround* popup menu selects the brightness of the area surrounding the specimen.

Weighting Factors

These are the default weighting factors used by the different difference equations for computing the ΔE CMC, ΔE 1994 and ΔE 2000 values.

Thresholds

Pass/Fail Metric

This sets the default metric to use for the Pass/Fail indicator. Choose from dE(ab), dE(CMC), dE94, dE00 and dCCT. The lowercase d here represents the Δ symbol.

ΔE , CIE XYZ, CIELAB 1976, CIELUV 1976, CIECAM02, Photometry, Density

These are the Pass/Fail thresholds for the various colorimetric differences.

SEARCH PREFERENCES

Search Tolerance

This is the default tolerance value which determines whether a test specimen's spectrum matches to the reference specimen's spectrum.

Spectral Graph

Grid


Chooses to show a grid and its color for the spectral search graph.

Background

Sets the default background color for the spectral search graph.

Line

Sets the default line color and width for drawing the spectral search graph.

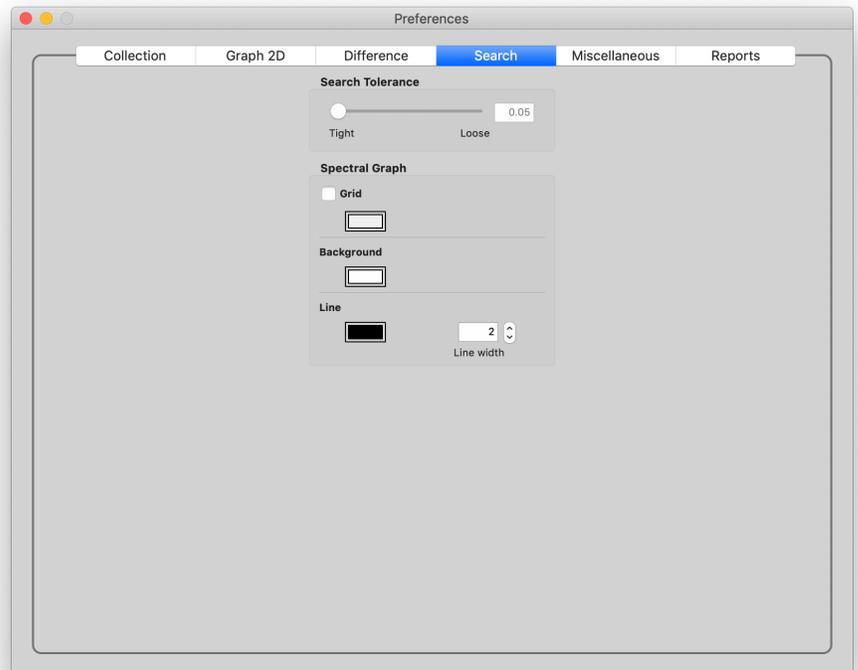

MISCELLANEOUS PREFERENCES

PR-655/670 Reference White Calibration

Click the *Open* button to load the reference data for the white calibration tile to be used with a PR-655 or PR-670 for reflective measurements. This file is a standard SpectraShop collection file with a **single** specimen.

Light Source Threshold

This value is used for transmissive calibration with any device that SpectraShop supports transmissive measurements. It is used for determining when the illumination is too low to be reliable. It is also used with the PR-655/670 for reflective measurements.


Monitor

SpectraShop does not use ICC profiles for displaying the simulated colors. Instead it uses a simple matrix RGB model. Here is where the colorimetric values for the monitor are specified.

Select one of the predefined monitor spaces or select *Custom* to specify your own values.

Selecting *Custom* permits setting the patch simulations to be more accurate when the monitor's white point and primaries are not one of the standard RGB spaces.

Enter the monitor's gamma value and the x, y coordinates for the monitor's three primaries and its white point. The conversion matrix will be automatically calculated when the *Preference* window is closed.

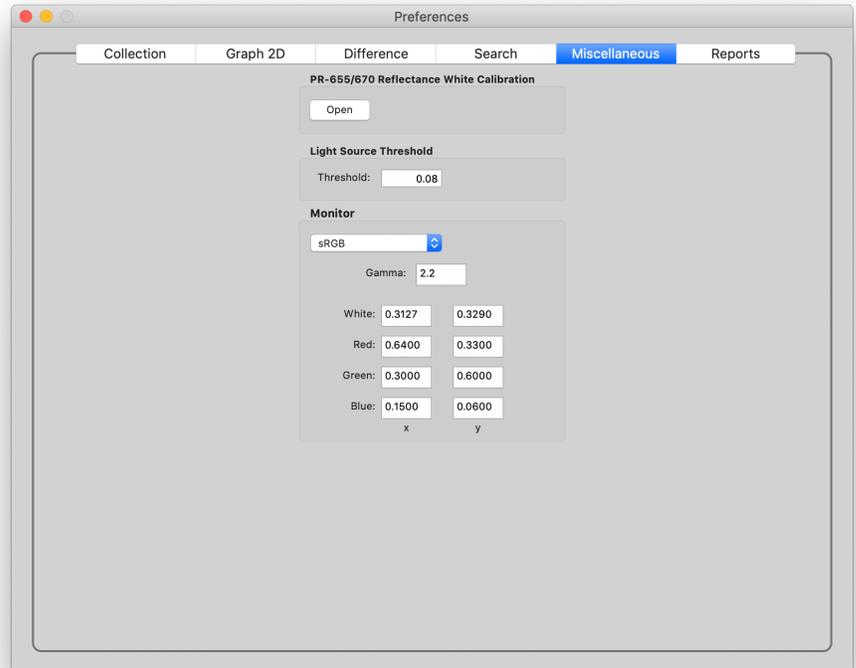

REPORTS PREFERENCES

Use Logo Image


Collection reports have an area reserved where a user specified logo may be printed on each report page.

The logo image must be either JPEG or PNG for a Macintosh, TIFF or GIF for a Windows machine.

SAVING PREFERENCES

The preferences are automatically saved when the *Preferences* window is closed.

Note: The preference file contains the actual data for the PR-655/670 white reference, so there is no need to reopen the reference file if it is moved to a different storage location.

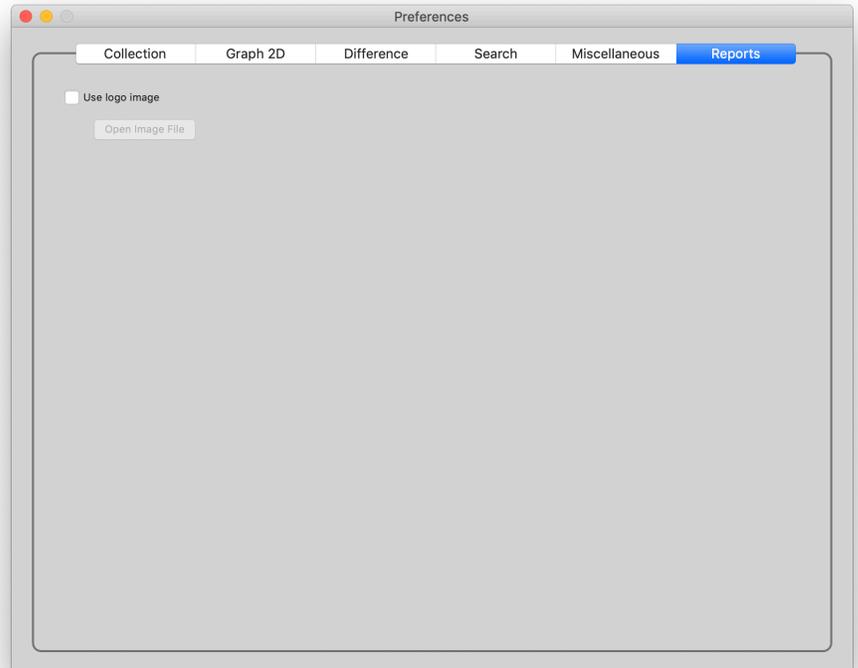

APPENDIX A - SUPPORTED INSTRUMENTS

DIRECTLY SUPPORTED INSTRUMENTS

The directly supported measuring instruments are listed in the table below along with some of their capabilities. Only **one** instrument at a time can be connected to SpectraShop. Spectra measured with the connected instrument are sent to the front-most collection window.

Instrument	ColorEye XTH	FD-7	i1Pro	i1Pro2	i1Pro3	i1Pro3 Plus	PR-655	PR-670	Spectrolino
Manufacturer	X-Rite	Konica-Minolta	X-Rite	X-Rite	X-Rite	X-Rite	Photo Research	Photo Research	GretagMacbeth
Emissive-Light		•	•	•	•	•	•	•	•
Emissive-Monitor			•	•	•	•	•	•	•
Emissive-Flash			•	•					
Reflective	•	•	•	•			• 1	• 1	•
Transmissive			• 1	• 1	• 1	• 1	• 1	• 1	• 1
Min. nm	360	360	380	380	380	380	380	380	380
Max. nm	750	730	730	730	730	730	780	780	730
Inc. nm	10	10 refl., 5 emis.	10	10	10	10	4	2	10
Geometry	Sphere	45/0	45/0	45/0	45/0	45/0			45/0
Apertures	5, 10 mm	3.5 mm	4 mm	4 mm	4 mm	4 mm	1 deg.	1, 0.5, 0.25, 0.125 deg.	4 mm
Filters	None	Ambient	Ambient ² , UV Cut ³	Ambient	Ambient	Ambient, Polarizer	Neutral density	Neutral density	Null, UV Cut, D65, Polarizer

1. This functionality is provided by SpectraShop, not the instrument.
2. Not available on i1Pro Rev. A.
3. UV Cut filter is a factory installed option for revisions A through D, not user replaceable.

X-RITE COLOREYE® XTH

The ColorEye XTH is a portable integrating sphere instrument manufactured by GretagMacbeth, now part of X-Rite. The omni-directional illumination and spectral capture of the integrating sphere makes it well suited to measuring textured surfaces, such as fabrics, in addition to smoother items. It has the ability to measure with the specular component included (SCI), excluded (SCE) or both simultaneously (SCI & SCE).

Note: When both the specular component included and excluded are chosen for simultaneous reporting, each geometry will be entered into the collection separately, generating two specimens for each item measured. **Multiple samples per specimen is disabled for this mode.**

The ColorEye® XTH uses an RS-232 hardware communication channel. A serial/USB adapter must be used with more recent computers that do not offer serial ports.

MINOLTA FD-7

This device measures both reflective and emissive-light specimens. When measuring reflective specimens, the instrument offers M0 (Illuminant A), M1 (Illuminant D50) and M2 (Illuminant A, UV excluded) measurement conditions. The instrument is a 45/0 geometry for reflective measurements. It also has the ability to scan patch strips for printer color management profile creation.

Note: SpectraShop does not currently support strip measurements for the FD-7.

Calibrating the FD-7 requires the use of the stapler attachment for all calibrations, including emissive-light. After clicking “Calibrate” in the Instrument window, place the FD-7 on the white plaque and press the stapler down to calibrate. Hold it there until the instrument signals the calibration is complete by beeping once.

Emissive-light measurements make use of the FD-7’s ambient diffuser. After calibration, replace the stapler attachment with the ambient filter. Click the “Start” button in the Measure Emissive-light window, aim the device then click the instrument’s “Scan/Illuminance” button to make each measurement.

UV Cut Reflective Measurements

When operating with the M2 measurement condition (UV excluded), a filter is employed internally to cut light emission below 400 nm. However, the FD-7 produces values in the 380-400 nm region. Although this is permitted by some measurement standards, having values here may lead the user to erroneous conclusions. For this reason, SpectraShop sets these values to zero. The UV Cut illumination condition M2 affects reflective measurements only.

Emissive-light Measurements

The FD-7 spectral output is in 10 nm increments for reflective measurements. For emissive-light measurements the spectral output is in 5 nm increments. This can be very helpful for light sources with narrow band emissions, such as fluorescent, HMI, HID or other sources utilizing mercury vapor emissions.

X-RITE I1PRO1, I1PRO2, I1PRO3

This handheld device is a 45/0 instrument manufactured by X-Rite. It can be ordered with a factory installed UV blocking filter for removing the effects of UV brighteners from reflective measurements. The only user replaceable filter is the ambient filter, used for measuring emissive light sources.

It has a variety of adapters which allow the i1Pro to measure emissive lights and flash (with the ambient filter), emissive monitors (with the counter-balanced monitor holder), reflective items with the spot adapter, strip charts with its strip measure ruler and emissive digital projectors with the beamer holder.

For automatic reflective chart measurement the i1Pro can be attached to the iO, an automated arm device.

Note: SpectraShop does not currently support strip measurements or the iO.

I1Pro Variations

The i1Pro has undergone five revisions; A, B, D, E (aka i1Pro 2), and i1Pro3 with some differences in the measurement capabilities between the revisions.

SpectraShop will automatically detect the revision of the connected i1Pro, setting the available measurement types in the Type popup menu.

Note: SpectraShop supports multiple i1Pro units attached to the computer, but **only one may be used at a time** to make spectral measurements. The instruments are differentiated by their serial numbers in the Spectrometer popup menu.

I1Pro Filters

UV-Cut

The i1Pro revisions A through D can be ordered with a factory installed UV Cut filter. This filter is used for measuring reflective prints without activating the optical brighteners in the paper. This is accomplished by filtering out the UV component of the instrument's illumination. Without UV illumination the paper's optical brightening agent will not fluoresce. The presence of this filter on the instrument is automatically detected and entered in the Measurement Data section for reflective measurements.

The i1Pro Rev. E, also known as the i1Pro 2, and the i1Pro3 have a user selectable UV Cut filter capability built into the instrument. This capability is selected as Illuminant M2.

Note: Although the UV Cut filter removes the UV component (380 to 400 nm) from the illumination, the i1Pro has an interpolation algorithm which attempts to fill the region from 380 to 400 nm with values. Putting estimated values into the spectrum is not appropriate because without illumination in this spectral region there should be no light energy to measure so the values would be expected to be zero. Another effect of the estimation algorithm is that these values can vary widely in magnitude from

measurement to measurement on the same specimen. Since this behavior can cause problems with some programs, SpectraShop corrects the values for 380 and 390 nm to zero to make it easier to work with the spectra in other programs. **This affects reflective measurements only.**

Ambient

There is only one user replaceable filter available for the i1Pro, revisions B through E, and the i1Pro3, the Ambient filter. The i1Pro Revision A did not have an ambient filter.

This filter is used for taking measurements of ambient light, light sources and photographic flashes. It is a diffusion filter that can be user installed. Select *Emissive-Light* from the *Type* popup menu and the *Ambient* filter will be automatically selected in the *Filter* popup menu.

Polarizer

The i1Pro3 Plus, the version with the 8 mm measurement aperture, also offers a replaceable polarization filter. This filter polarizes the light before it interacts with the subject's surface, then it has a second polarizer, rotated 90 degrees from the first, in front of the light measurement optics. The result is that any specular reflection from the surface of a glossy subject is removed from the measured spectrum. Using a polarization filter is also referred to as measurement condition M3.

Note: This polarization filter is only available on the 8 mm aperture, also known as the "large aperture" or "LA" instrument or as the i1Pro3 Plus. The 4 mm aperture i1Pro3 instrument, also called the "small aperture", or "SA" instrument does not have this filter available.

Measurement Modes

With the i1Pro 2 (also known as the i1Pro Rev. E) and the i1Pro3, the instrument now has user selectable lighting conditions for reflective measurements. These conditions are selected with the Illuminant popup menu. M0 is tungsten illumination, which contains a small amount of UV light. M1 is a combination of tungsten illumination combined with a UV LED, then processed to give a D50 illumination. M2 is tungsten with a UV-Cut filter. This is the same condition as a revision A through D instrument with a UV cut filter installed.

PHOTO RESEARCH PR-655 & PR-670

These two instruments are portable spectroradiometers. Using a design similar to a camcorder, the instrument is pointed at an object and whatever is beneath a black spot visible in the eyepiece is spectrally measured. They both offer a wide range of interchangeable lenses, filters and accessories which allow them to measure almost anything emissive, reflective or transmissive. For reflective measurements the user must supply their own lighting and a reflective reference target (e.g. Spectralon® or Fluorinon® 99% reflective white tile). For transmissive measurements the user must also supply a lighting setup.

Currently, the only Photo Research accessories supported by SpectraShop are the MS-75 primary lens and the CR-650 or CR-670 cosine correctors used for ambient light measurements.

X-RITE SPECTROLINO

This handheld device is a 45/0 instrument manufactured by GretagMacbeth, now part of X-Rite. It was the predecessor to the i1Pro.

It has a variety of adapters which allow the Spectrolino to measure emissive monitors (with the counter-balanced monitor holder) and reflective items with the spot adapter.

For automatic reflective chart measurement the Spectrolino can be attached to the SpectroScan, an automated stage.

Note: SpectraShop does not currently support using the Spectrolino with the SpectroScan automated stage.

Spectrolino Filters

Filters are used to adjust the measurement characteristics of a spectrophotometer to improve its results. The available Spectrolino filters are Null, D65, Polarizer and UV Cutoff.

The filters attach over the measuring head, the portion of the instrument where both the illumination and the sensor aperture are located. The Spectrolino illuminates the specimen with an annular 45 degree beam. This means the light is coming from a 360 degree circle around the center of the measuring head, oriented so the light arrives at the specimen from a 45 degree angle from the plane of the specimen.

The Spectrolino filters perform two functions; to adjust the spectrum of the illumination, and to modify the sensor's response. To achieve these functions, some filters have two distinct regions. The outer portion of the round filter is used to adjust the illumination, the filter's center area contains the sensor filter. By looking at the filter at an angle from the back side, the two filter region's can be observed.

Null

This is the most commonly used filter on the Spectrolino. It is marked with a "U". It is used for Illuminant A measurements and for all emissive and transmissive measurements. It is a clear glass filter that does not alter the illumination or measurement spectra. It is, however, necessary to maintain a common physical configuration of the instrument for measurements with the other filters.

D65

The illumination source in the Spectrolino is a tungsten lamp. The lamp emits a small amount of light at the violet wavelengths and a high amount of red light. Silicon sensors are more sensitive to red and infrared light than to ultraviolet and blue lights. This means that for the blue end of the spectrum, a larger scale factor is necessary to normalize the spectral data when reference illuminants that contain more blue light are selected for the measurements.

The D65 filter cuts back on the red end of the illumination and passes more blue light. This evens out the scale factors and evens the error distribution for the spectrum. Since less light is illuminating the specimen, the Spectrolino will take a longer time measuring the spectrum to increase the signal and improve the signal to noise ratio for the measurement.

Polarizer

When making measurements of glossy surfaces, a small amount of light will be polarized and reflect from the surface toward the sensor, thus altering the measured color.

The polarizing filter has an outer portion that polarizes the illumination and an inner portion set at a 90° rotation from the outer. The result is that the specular reflection from the surface is polarized by the outer portion and the inner portion will block this light, thus letting the instrument measure only the color. When the light is polarized, the full intensity is not transmitted through the filter. Typical polarizers pass only 38% of the light. The combined effect of polarization will then only transmit about 14% of the original illumination ($0.38 \times 0.38 = 0.14$).

Due to this light loss, the Spectrolino will increase the measuring time to get an adequate signal to noise ratio when the polarizing filter is used.

UV Cut

This filter is most often used with substrates that have optical brighteners. Most white “plain” papers use brighteners to convert invisible ultraviolet light to visible blue light, thus offsetting the natural yellowness of paper fibers. Optical brighteners are also used in the fabric industry to offset the natural yellow color of textile fibers and the increasing yellowness that occurs as the fabric ages. This extra blue reflectance can cause problems with creating color management profiles, producing profiles that generate a yellow cast in the images to compensate for the bluishness of the paper.

The UV Cut filter is designed to remove ultraviolet light from the illumination, thus eliminating the blue fluorescence. The outer portion of the filter is yellow and removes the ultraviolet light from the illumination. The inner portion is blue to improve the measurement in the blue end of the spectrum to offset the decreased blue illumination. Again, the integration time is slightly longer to improve the signal to noise ratio.

APPENDIX B – CHART DEFINITION FILE FORMAT

The file is an ASCII text file containing a sequence of lines consisting of one or more keywords followed by other keywords or the corresponding parameters and data. A line is terminated by the carriage return character. Each keyword is separated from its parameter by white space consisting of either a **tab** or a **space** character. A tab character is recommended for easier formatting in word processing programs.

Required keywords for all chart types

Keyword	Parameter	Explanation
SpectraShop Chart	version number	"5" for this release. Signifies the standard used for the file encoding. Must be the first item in the file.
SPECIMEN_ID	string	Identifies the specimen.
SPECTRUM_TYPE	string, one of: "emissive_monitor" "reflective" "transmissive"	
MANUFACTURER	string	Manufacturer of the chart.
MATERIAL	string	Composition of the patches.
NUMBER_OF_PATCHES	integer	Number of patches contained in the chart.
CHART_UNITS	string, one of: "IN" "CM"	Identifies the units used for positions and sizes. Required for reflective and transmissive charts.
CHART_WIDTH	float	Horizontal size of the chart from the defined chart origin.
CHART_HEIGHT	float	Vertical size of the chart from the defined chart origin.
BEGIN_DATA_FORMAT		Marks the beginning of the list of data value identifiers.
END_DATA_FORMAT		Marks the end of the list of data value identifiers.
BEGIN_DATA		Marks the beginning of the data value list defined by the data value identifier list and the NUMBER_OF_SETS data keyword.

END_DATA		Marks the end of the data value list.
SURFACE	string one of: "matte" "semi-gloss" "gloss" "metallic" "interference" "na"	Type of surface for a reflective specimen.
PATCH_LEFT	float	Horizontal position for the upper-left corner of the patch from the defined chart origin, in millimeters.
PATCH_TOP	float	Vertical position for the upper-left corner of the patch from the defined chart origin, in millimeters.
PATCH_WIDTH	float	Horizontal size of the patch, in millimeters.
PATCH_HEIGHT	float	Vertical size of the patch, in millimeters.
ID	string	Identifies the chart patch.

Required keywords for XY table charts

Keyword	Parameter	Explanation
CHART_UPPER_LEFT	string	Message to the operator defining the chart origin.
CHART_LOWER_LEFT	string	Message to the operator defining the chart's vertical extent.
CHART_UPPER_RIGHT	string	Message to the operator defining the chart's horizontal extent.
CHART_LOWER_RIGHT	string	Message to the operator defining the chart's horizontal extent.

Optional keywords

Keyword	Parameter	Explanation
#	string	Comment identifier. Any data until the next end-of-line character is ignored by the automatic reader.
CHART_NAME	string	Identifies the chart.

CHART EXAMPLE 1, EMISSIVE-MONITOR

SpectraShop 5 Chart

CHART_TYPE "Emissive_monitor"

CHART_NAME "RGB 8 Primaries"

#

BEGIN_DATA_FORMAT

ID RGB_R RGB_G RGB_B

END_DATA_FORMAT

#

NUMBER_OF_SETS 8

BEGIN_DATA

"R000-G000-B000"	0	0	0
"R255-G000-B000"	255	0	0
"R000-G255-B000"	0	255	0
"R255-G255-B000"	255	255	0
"R000-G000-B255"	0	0	255
"R255-G000-B255"	255	0	255
"R000-G255-B255"	0	255	255
"R255-G255-B255"	255	255	255

END_DATA

CHART EXAMPLE 2, REFLECTIVE

SpectraShop 5 Chart

```
CHART_TYPE      "Reflective"
CHART_NAME      "ColorChecker Classic"
CHART_UNITS     "IN"
CHART_WIDTH     11.375
CHART_HEIGHT    8
```

Name	380	390	400	...	770	780
Sample 1	0.1958	0.2011	0.2012		0.5962	0.6042
Sample 2	0.2330	0.2443	0.2422		0.6595	0.6666
...						
Sample n	0.1487	0.1571	0.1581		0.5635	0.5738

```
UL_DESCRIPTION "Mark the upper-left corner of the Dark skin patch"
UR_DESCRIPTION "Mark the upper-right corner of Bluish green."
LL_DESCRIPTION "Mark the lower-left corner of the White patch"
LR_DESCRIPTION "Mark the lower-right corner of the Black patch"
MANUFACTURER  "X-Rite"
MATERIAL      "Paint"
```

#

BEGIN_DATA_FORMAT

```
ID    SURFACE    PATCH_LEFT    PATCH_TOP    PATCH_WIDTH    PATCH_HEIGHT
```

END_DATA_FORMAT

#

NUMBER_OF_SETS 24

BEGIN_DATA

```
"Dark skin"      "matte"    0.388        0.5  1.6  1.6
"Light skin"     "matte"    2.188        0.5  1.6  1.6
"Blue sky"       "matte"    3.988        0.5  1.6  1.6
"Foliage"        "matte"    5.788        0.5  1.6  1.6
"Blue flower"   "matte"    7.588        0.5  1.6  1.6
"Bluish green"  "matte"    9.388        0.5  1.6  1.6
"Orange"        "matte"    0.388        2.3  1.6  1.6
"Purplish blue" "matte"    2.188        2.3  1.6  1.6
"Moderate red"  "matte"    3.988        2.3  1.6  1.6
"Purple"        "matte"    5.788        2.3  1.6  1.6
"Yellow green"  "matte"    7.588        2.3  1.6  1.6
"Orange yellow" "matte"    9.388        2.3  1.6  1.6
"Blue"          "matte"    0.388        4.1  1.6  1.6
"Green"         "matte"    2.188        4.1  1.6  1.6
"Red"           "matte"    3.988        4.1  1.6  1.6
"Yellow"        "matte"    5.788        4.1  1.6  1.6
"Magenta"       "matte"    7.588        4.1  1.6  1.6
"Cyan"          "matte"    9.388        4.1  1.6  1.6
"White"         "matte"    0.388        5.9  1.6  1.6
"Neutral 8"     "matte"    2.188        5.9  1.6  1.6
```

"Neutral 6.5"	"matte"	3.988	5.9	1.6	1.6
"Neutral 5"	"matte"	5.788	5.9	1.6	1.6
"Neutral 3.5"	"matte"	7.588	5.9	1.6	1.6
"Black"	"matte"	9.388	5.9	1.6	1.6

END_DATA

APPENDIX C – SPECTRASHOP 6 IMPORT/EXPORT TEXT FORMAT

The file is a text file containing a sequence of lines consisting of one or more keywords followed by other keywords or the corresponding parameters and data. A line is terminated by a carriage return character and a linefeed character. Each keyword is separated from its parameter by white space consisting of a tab character. The tab character makes it easier to process the file in spreadsheet or text editing programs.

FILE STRUCTURE

The file is composed of three parts: a file header, measurement metadata, specimen data.

Part 1: The file header consists of keywords and parameters which apply to the entire collection contained within the file.

Part 2: The next section contains the measurement metadata in common to all the specimens within the following specimen section.

Part 3: The third section consists of the metadata and data for each specimen.

Whenever a metadata item in the measurement metadata changes, a new Part 2 is written, followed immediately by the associated Part 3 specimens. Thus Parts 2 and 3 are repeated until all the specimens within the collection are written.

Example: a collection consisting of reflective specimens followed by emissive-light specimens would be represented in the file as the file header, then the reflective measurement metadata, the reflective specimens, the emissive-light measurement metadata followed by the emissive-light specimens.

File Header Section
Metadata Section 1
Data Section 1
...
Metadata Section n
Data Section n

Import/Export file layout

File Section Keywords

Keyword	Parameter	Required ?	Description
SpectraShop	3.0	Yes	Signifies the standard used for the file encoding. Must be the first item encountered in the file.
FILE_DESCRIPTOR	string		Description of the purpose or content of the record.
NUMBER_OF_SETS	integer	Yes	Number of specimens in the file.

Metadata Section Keywords

Keyword	Parameter	Required ?	Description
#			Comment identifier. Any data until the next end-of-line characters is ignored by the file reader.
ACQUIRE_NOTE	string		Note relating to the spectra acquisition.
BEGIN_DATA_FORMAT		Yes	Marks the beginning of the list of data value identifiers.
CREATED	date string		Date the spectra were created or measured.
END_DATA_FORMAT		Yes	Marks the end of the list of data value identifiers.
ILLUMINANT	string	Note 1	Defines the illuminant used for calculating colorimetric values for reflective and transmissive specimens.
INSTRUMENTATION	string		Instrument used to make the spectral measurements.
MANUFACTURER	string		Manufacturer of the specimens.
MATERIAL	string		Composition of the specimens.
MEASUREMENT_GEOMETRY	string		Geometry of the instrument used to make the spectral measurements.
MEASUREMENT_SOURCE	string		Light source used with the instrument to make the spectral measurements.
MEASUREMENT_APERTURE	string		Instrument's measurement aperture size, usually expressed in millimeters.
MEASUREMENT_FILTER	string		Filter used on the spectrophotometer during the measurements.

MODEL	string		Model number, if applicable, for the specimens.
NMEASURE	integer		Number of measurements per specimen.
NOTE	string		Notes relating to the specimens.
NUMBER_OF_FIELDS	integer	Yes	Must precede the BEGIN_DATA_FORMAT keyword. Number of data format identifiers prescribed in the data format definition that follows.
OBSERVER	string	Note 1	Defines the standard observer used for calculating the colorimetric values.
ORIGINATOR	string		Specific system, organization, or individual originating the spectra.
PROD_DATE	date string		Date when the specimens were manufactured.
RGB_SPACE	string	Note 2	Defines the RGB space used for calculating RGB values.

Keyword	Parameter	Required ?	Description
SAMPLE_BACKING	string		Backing used behind reflective samples during the measurement.
SERIAL	string		Serial number, if applicable, for the object being measured.
SPECTRUM_TYPE	string	Yes	Signifies the standard used for the file encoding. Must be the first item encountered in the file.
SURFACE	string		Type of surface for a reflective specimen.

Note 1: Required for colorimetric data export. Note 2: Required for RGB data export.

Data Format Keywords

Keyword	Associated Data Value	Required ?	Description
CCT	float		Correlated Color Temperature. Emissive light or monitor value.
CD	float		Cd/m ² . Emissive monitor radiance.
DOM_NM	float		Dominant wavelength.
ISO1	float		ISO1 density value.

ISO1	float		ISO2 density value.
JCH_A	float		CIECAM02 a* value. Redness-greenness.
JCH_B	float		CIECAM02 b value. Yellowness-blueness.
JCH_C	float		CIECAM02 C* value. Chroma.
JCH_H	float		CIECAM02 H* value. Hue angle, in degrees.
JCH_J	float		CIECAM02 J* value. Lightness.
LAB_A	float		CIELAB 1976 a* value. Redness-greenness.
LAB_B	float		CIELAB 1976 b* value. Yellowness-blueness.
LAB_C	float		CIELAB 1976 C* value. Chroma.
LAB_H	float		CIELAB 1976 h value. Hue angle, in degrees.
LAB_L	float		CIELAB 1976 L* value. Lightness.
LUV_C	float		CIELUV 1976 C* value. Chroma.
LUV_H	float		CIELUV 1976 h value. Hue angle, in degrees.
LUV_L	float		CIELUV 1976 L* value. Lightness.
LUV_S	float		CIELUV 1976 s value. Saturation.
LUV_U	float		CIELUV 1976 u* value. Redness-greenness.
LUV_V	float		CIELUV 1976 v* value. Yellowness-blueness.
LUX	float		Lux. Emissive light illuminance.
PE	float		Excitation purity.
RGB_B	integer		RGB blue value.
RGB_G	integer		RGB green value.
RGB_R	integer		RGB red value.
RGB_OUT_OF_GAMUT	string		RGB clipped? Value is "True" or "False".
SAMPLE_ID1	string	Yes	First specimen identifier.

Keyword	Associated Data Value	Required ?	Description
SAMPLE_ID2	string		Second specimen identifier.
SAMPLE_ID3	string		Third specimen identifier.
SPECTRAL_END	integer	Note 1	Ending wavelength for the specimen spectra.
SPECTRAL_INC	integer	Note 1	Width of each band for the specimen spectra.

SPECTRAL_START	integer	Note 1	Starting wavelength for the specimen spectra.
SPECTRAL_SUM	float		Sum of spectral bands, approximate integral.
SPECTRAL_VAL	float	Note 1	Denotes a spectral value for a measurement band. For non-fluorescing reflective and transmissive spectra the data is in the range 0-1. For emissive specimens the data is in $W/(m^2 sr nm)$.
STATUS_A_B	float		Status A blue density.
STATUS_A_G	float		Status A green density.
STATUS_A_R	float		Status A red density.
STATUS_E_B	float		Status E blue density.
STATUS_E_G	float		Status E green density.
STATUS_E_R	float		Status E red density.
STATUS_I_B	float		Status I blue density.
STATUS_I_G	float		Status I green density.
STATUS_I_R	float		Status I red density.
STATUS_M_B	float		Status M blue density.
STATUS_M_G	float		Status M green density.
STATUS_M_R	float		Status M red density.
STATUS_T_B	float		Status T blue density.
STATUS_T_G	float		Status T green density.
STATUS_T_R	float		Status T red density.
STATUS_V	float		Visual density.
UV_U	float		1964 u' value.
UV_V	float		1964 v' value.
WATTS	float		$W/(m^2 sr)$. Emissive light or monitor intensity.
XYY_X	float		Chromaticity x value.
XYY_Y	float		Chromaticity y value.
XYY_CAPY	float		Chromaticity Y value, same as XYZ_Y.
XYZ_X	float		Tristimulus X value.
XYZ_Y	float		Tristimulus Y value.
XYZ_Z	float		Tristimulus Z value.

Note 1: Required for a SpectraShop import file.

Specimen Data Keywords

Keyword	Parameter	Required ?	Description
BEGIN_DATA		Yes	Marks the beginning of the specimen data list defined by the data format list and the NUMBER_OF_SETS data keyword.
END_DATA		Yes	Marks the end of the specimen list.

Keyword Parameters

Keyword	Parameter Values
ILLUMINANT	Select one of: "A", "C", "D50", "D55", "D65", "D75", "E", "F1", "F2", "F3", "F4", "F5", "F6", "F7", "F8", "F9", "F10", "F11", "F12"
MEASUREMENT_FILTER	Examples: "Polarizer", "UV Block"
MEASUREMENT_GEOMETRY	Examples: "45/0", "d/0", "d/8 SCI"
OBSERVER	Select one of: "2 degree", "10 degree"
RGB_SPACE	Examples: "Adobe RGB", "sRGB", "Wide Gamut"
SAMPLE_BACKING	Examples: "Black", "White", "Substrate", "Self"
SPECTRUM_TYPE	Select one of: "Emissive-light", "Emissive-monitor", "Reflective", "Transmissive"
SURFACE	Examples: "Matte", "Semigloss", "Gloss", "Metallic"

Parameter and Data Values

Parameter or Value type	Description
date string	A series of numeric characters 0 through 9, inclusive, with separating hyphen characters and representing the ISO 8601 format YYYY-MM-DD. Example: 2001-01-25 is 25 January 2001

float	<p>A combination of numeric characters 0 through 9, the decimal point character (.) and optionally including an exponent consisting of an E character with either a plus (+) or a minus (-) character. The data should include a decimal point character. A decimal point will be assumed at the end of the number if it does not contain one. Numbers less than 1 must contain a leading 0 and decimal point.</p> <p>Examples:</p> <p>10.45 0.3456 1.2345E+1 2.4567E-2 1.2345E1</p>
integer	<p>A combination of numeric characters 0 through 9, inclusive, without a decimal point or other alphanumeric characters.</p> <p>Example: 123</p>

Parameter or Value type	Description
string	<p>A series of alphanumeric characters enclosed within quote (") characters. Quote characters are not allowed within the string. The first occurrence of a quote within the string terminates the string, thus, the use of the double-quote to denote a single quote character (C language syntax) is not supported.</p> <p>Example: "this is a string"</p>

Items Requiring New Metadata Section Definition

This table lists the keywords that when their values change within a collection a new metadata section must be written to the import/export file.

Keyword
ACQUIRE_NOTE
CREATED
INSTRUMENTATION
MANUFACTURER
MATERIAL
MEASUREMENT_GEOMETRY
MEASUREMENT_SOURCE
MEASUREMENT_APERTURE
MEASUREMENT_FILTER
MODEL

NMEASURE
NOTE
ORIGINATOR
PROD_DATE
SAMPLE_BACKING
SERIAL
SPECTRAL_END
SPECTRAL_INC
SPECTRAL_START
SPECTRUM_TYPE
SURFACE

EXAMPLE 1

This file illustrates a file with a single reflective specimen. All keywords and values are separated by tab characters. Each line ends with a carriage return character and a linefeed character. Notice that exponential notation is used to maintain numeric values over a wider range than a simple value.

```
SpectraShop      5.0
FILE_DESCRIPTOR  "Theoretical 18% gray reference."
NUMBER_OF_SETS  1
ORIGINATOR      "Robin D. Myers"
CREATED         "2001-04-13"
SPECTRUM_TYPE   "Reflective"
SURFACE         "Matte"
INSTRUMENTATION "Reference"
INSTRUMENT_SERIAL_NUMBER ""
MEASUREMENT_GEOMETRY "45/0"
MEASUREMENT_SOURCE "A"
MEASUREMENT_APERTURE ""
MEASUREMENT_FILTER "None"
SAMPLE_BACKING  "Black"
NSAMPLES        1
OBSERVER        "10 degree"
ILLUMINANT      "D65"
RGB_SPACE       "Adobe 1998"
NUMBER_OF_FIELDS 75
BEGIN_DATA_FORMAT
SAMPLE_ID1      SAMPLE_ID2      SAMPLE_ID3      SPECTRAL_NM      SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
END_DATA_FORMAT
BEGIN_DATA
"18% Gray aim point"      ""      ""
380  1.800000E-1
390  1.800000E-1
400  1.800000E-1
410  1.800000E-1
420  1.800000E-1
```

430 1.800000E-1
440 1.800000E-1
450 1.800000E-1
460 1.800000E-1
470 1.800000E-1
480 1.800000E-1
490 1.800000E-1
500 1.800000E-1
510 1.800000E-1
520 1.800000E-1
530 1.800000E-1
540 1.800000E-1
550 1.800000E-1
560 1.800000E-1
570 1.800000E-1
580 1.800000E-1
590 1.800000E-1
600 1.800000E-1
610 1.800000E-1
620 1.800000E-1
630 1.800000E-1
640 1.800000E-1
650 1.800000E-1
660 1.800000E-1
670 1.800000E-1
680 1.800000E-1
690 1.800000E-1
700 1.800000E-1
710 1.800000E-1
720 1.800000E-1
730 1.800000E-1
END_DATA

EXAMPLE 2

This file illustrates a file with two specimens; a single reflective specimen and a single emissive light specimen. Since the spectrum type changes from the first to the second specimen a new metadata section is written for the second specimen. Also note that the data format declaration changes for the emissive light specimen. The “ICCT” data was selected in the Export window, but since that does not apply to reflective specimens it is not included in the first metadata section but it is included for the emissive light specimen’s metadata section. These two specimens have different sampling increments, which is one special SpectraShop feature.

```
SpectraShop      5.0
FILE_DESCRIPTOR  "Theoretical 18% gray reference."
NUMBER_OF_SETS  2
ORIGINATOR      "Robin D. Myers"
CREATED         "2001-04-13"
SPECTRUM_TYPE   "Reflective"
SURFACE         "Matte"
INSTRUMENTATION "Reference"
INSTRUMENT_SERIAL_NUMBER ""
MEASUREMENT_GEOMETRY "45/0"
MEASUREMENT_SOURCE "A"
MEASUREMENT_APERTURE ""
MEASUREMENT_FILTER "None"
SAMPLE_BACKING  "Black"
NSAMPLES        1
OBSERVER        "10 degree"
ILLUMINANT      "D65"
RGB_SPACE       "Adobe 1998"
NUMBER_OF_FIELDS 75
BEGIN_DATA_FORMAT
SAMPLE_ID1      SAMPLE_ID2      SAMPLE_ID3      SPECTRAL_NM      SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM
SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL     SPECTRAL_NM     SPECTRAL_VAL
END_DATA_FORMAT
BEGIN_DATA
"18% Gray aim point"      ""      ""
380  1.800000E-1
```

390 1.800000E-1
400 1.800000E-1
410 1.800000E-1
420 1.800000E-1
430 1.800000E-1
440 1.800000E-1
450 1.800000E-1
460 1.800000E-1
470 1.800000E-1
480 1.800000E-1
490 1.800000E-1
500 1.800000E-1
510 1.800000E-1
520 1.800000E-1
530 1.800000E-1
540 1.800000E-1
550 1.800000E-1
560 1.800000E-1
570 1.800000E-1
580 1.800000E-1
590 1.800000E-1
600 1.800000E-1
610 1.800000E-1
620 1.800000E-1
630 1.800000E-1
640 1.800000E-1
650 1.800000E-1
660 1.800000E-1
670 1.800000E-1
680 1.800000E-1
690 1.800000E-1
700 1.800000E-1
710 1.800000E-1
720 1.800000E-1
730 1.800000E-1

END_DATA

ORIGINATOR "Robin D. Myers"

CREATED "2011-03-01"

SPECTRUM_TYPE "Emissive-light"

SURFACE "N/A"

INSTRUMENTATION "Reference"

INSTRUMENT_SERIAL_NUMBER ""

MEASUREMENT_GEOMETRY "0/d"

MEASUREMENT_APERTURE ""

MEASUREMENT_FILTER ""

NSAMPLES 1

OBSERVER "10 degree"

ILLUMINANT "D65"

NUMBER_OF_FIELDS 165

BEGIN_DATA_FORMAT

455 3.540680E+1
460 3.781210E+1
465 4.030020E+1
470 4.286930E+1
475 4.551740E+1
480 4.824230E+1
485 5.104180E+1
490 5.391320E+1
495 5.685390E+1
500 5.986110E+1
505 6.293200E+1
510 6.606350E+1
515 6.925250E+1
520 7.249590E+1
525 7.579030E+1
530 7.913260E+1
535 8.251930E+1
540 8.594700E+1
545 8.941240E+1
550 9.291200E+1
555 9.644230E+1
560 1.000000E+2
565 1.035820E+2
570 1.071840E+2
575 1.108030E+2
580 1.144360E+2
585 1.180800E+2
590 1.217310E+2
595 1.253860E+2
600 1.290430E+2
605 1.326970E+2
610 1.363460E+2
615 1.399880E+2
620 1.436180E+2
625 1.472350E+2
630 1.508360E+2
635 1.544180E+2
640 1.579790E+2
645 1.615160E+2
650 1.650280E+2
655 1.685100E+2
660 1.719630E+2
665 1.753830E+2
670 1.787690E+2
675 1.821180E+2
680 1.854290E+2
685 1.887010E+2
690 1.919310E+2
695 1.951180E+2
700 1.982610E+2
705 2.013590E+2

710 2.044090E+2
715 2.074110E+2
720 2.103650E+2
725 2.132680E+2
730 2.161200E+2
735 2.189200E+2
740 2.216670E+2
745 2.243610E+2
750 2.270000E+2
755 2.295850E+2
760 2.321150E+2
765 2.345890E+2
770 2.370080E+2
775 2.393700E+2
780 2.416750E+2
END_DATA

APPENDIX D – SPREADSHEET IMPORT/EXPORT FORMAT

SpectraShop can import comma separated data from spreadsheets or generated from other programs.

Here is a portion of a spreadsheet showing how the original data must be formatted.

Here is how this data appears in the file.

```
Name,380,390,400, ...,770,780  
Sample 1,0.1958,0.2011,0.2012,...,0.5962,0.6042  
Sample 2,0.2330,0.2443,0.2422,...,0.6595,0.6666  
...  
Sample n,0.1487,0.1571,0.1581,...,0.5635,0.5738
```

This same format is used for SpectraShop’s spreadsheet export.

SpectraShop 6 supports a data range from 200 to 1100 nm, inclusive. The spectral sampling may be in 1, 2, 4, 5 or 10 nm bands. At 1 nm over the full range, this will result in 902 columns. Microsoft Excel can operate with up to 1024 columns, but other programs, such as Apple Numbers, have a 255 column limit.

While SpectraShop can operate for both importing and exporting in the spreadsheet format with more than 255 data values, it may make it difficult to open the file in a spreadsheet.

Note: This format does not allow for any metadata, so on import the specimens are assigned a “reflective” type. After import, use the Edit feature in the collection to change the type, if necessary, and to add any available metadata.

APPENDIX E – CONVERTING SPECTRASHOP 1 AND 2 FILES

SpectraShop 6 will read version 1 and 2 collection files, converting all the data with the exception of two items; emissive specimens and date formats.

SPECIMEN TYPE

Since version 3 now differentiates between emissive-light and emissive-monitor measurements, when version 1 or 2 collections are opened there is no way to decide which type for each emissive specimen. By default they will be tagged as emissive-monitor. To change this designation, select all the specimens that should be changed then click the *Edit Metadata* icon. The specimen type may then be changed.

DATE FORMAT

SpectraShop 1 and 2 treated all dates as strings. This allowed for any date format but it made a problem for converting them into the ISO 8601 date format used by SpectraShop 6. As a string the date may be expressed in a wide variety of formats. A few examples are below.

7 January 2004
January 7, 2004
1/7/2004
1/7/04
7.1.2004
7/1/2004
2004.1.7
2004 Jan. 7
7 Jan 2004

The problem can be seen in the examples above. It is impossible to tell the day from the month in short date formats when the day is less than 13. Dates such as 1/7/2004 and 7/1/2004 can be correctly interpreted as January 7 or July 1.

SpectraShop 6 opens the version 1 and 2 files without changing the date strings, but any new specimens will use the ISO 8601 date format of YYYY-MM-DD. This could cause some confusion when old and new specimens are mixed in the same collection, or if one date in a specimen was edited in version 3 but another date was in the original format.

It is highly recommended that dates should be checked and edited, if necessary, when version 1 and 2 collections are opened.

APPENDIX F – SPECTRAL DATA


Spectrometers measure data in a variety of sampling intervals and ranges. For instance, an X-Rite i1Pro reports the spectrum from 380 to 730 nm in 10 nm increments. A Photo Research PR-655 measures from 380 to 780 nm in 4 nm increments. To allow spectra from these two instruments to be used together, common range and data formats need to be established.

RANGE

When working with shorter ranges there are several possible ways to handle the data. One technique is to take the last data value and replicate it for the missing values until the end of the range is reached. For example, if the instrument's last value is 730 nm and the range must be extended to 780 nm, then the 730 nm value is copied into the value for 740 nm, then 750, and so forth, until 780 nm is reached, assuming a 10 nm sampling.

Another way to extend a range is to fit a mathematical function to the end of the spectrum and generate values from this function. The accuracy depends on the shape of the original spectrum and the function used. As the distance increases from the end of the actual data range the error in the extrapolated data usually increases.

The problem with copying data or extrapolating data is this generated data may not correlate with the actual spectral response of the specimen. Measurement noise can alter the extrapolating function resulting in extremely high errors in the extrapolated spectral regions. In the three spectra at the right, the same specimen was repeatedly measured with a spectrometer equipped with a UV-Cut filter which removes all illumination below 400 nm. Sensor noise has affected the instrument's interpolation routine, resulting in wildly varying reflectances in this region.

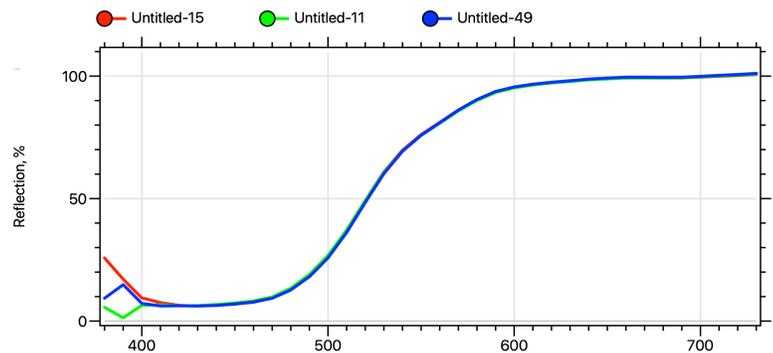

Perhaps the biggest problem with extrapolating or copying the data into regions the spectrometer does not report is that it **leads to false assumptions interpreting the spectrum.**

To prevent adding errors to the spectral data, SpectraShop extends spectral ranges by putting zero values into the missing range.

SAMPLING

The other major issue with spectra is the sampling interval. Most low-cost spectrometers sample the spectrum in 10 nm increments. More expensive instruments sample at 5, 4, 2 or 1 nm increments. Some of the standards for illuminants are specified in 5 nm increments while the CIE observers are tabulated in 1 nm increments. Comparing data between instruments with differing sample intervals can create problems. CIE Standard 15:2004 states that for “rigorous calculations” the data should be represented in 1 nm increments. To get 1 nm data from larger increment sampling (e.g. 10 nm) it is necessary to interpolate, or mathematically estimate the data between samples. While there are many possible methods to interpolate data (e.g. linear, polynomial, piece-wise polynomial) in CIE 167:2005 the Sprague interpolation, a fifth-degree polynomial, is the recommended method. It is designed to interpolate data which has fixed sampling intervals and it has the benefit that the interpolation curve passes through the original sample points.

SpectraShop uses the Sprague interpolation method to convert all data sampled at intervals greater than 1 nm into 1 nm data. It currently interpolates 1.3, 2, 4, 5 and 10 nm data.

With all specimen spectra using 1 nm sampling, and containing data in the range from 380 to 780 nm, inclusive, **spectra from almost any instrument may be freely compared and processed with data from other instruments.**

APPENDIX G – FREQUENTLY ASKED QUESTIONS (FAQ)

1. Why does my i1Pro not appear in the *Instrument* list in the Instrument window?

A. There may be several reasons. The most common is that there is another program which can access the i1Pro and it may have connected to the i1Pro before SpectraShop. Only one program may connect to an i1Pro at one time. Make sure the other programs are closed, then relaunch SpectraShop.

Another reason may be that your version of X-Rite Device Services (XRDS) needs updating. XRDS is a program installed by i1Profiler and possibly other X-Rite programs. When the OS version is updated, XRDS needs to be updated, as well. You will need to search the xrite.com website for this program.

Another reason is that the i1Pro may not have been registered by the operating system. Occasionally the OS may not recognize the instrument, so unplug the i1Pro, wait a few seconds, then replug it into the USB port. If the i1Pro is detected by SpectraShop it will appear in the *Instrument* popup menu.

Lastly, on Windows computers a device driver must be installed before the i1Pro is recognized by the OS. This driver is installed as part of the i1Profiler installation, and it might also be installed with the i1Diagnostics program, if you install this.

2. Why is the ColorMunki not one of the directly supported instruments?

A. X-Rite does not provide a set of libraries for connecting to the ColorMunki, nor does it provide the communication protocols. Use the *Import/File* menu to bring ColorMunki application measurement files into SpectraShop.

REFERENCES

In preparing SpectraShop™ 6 strict adherence to the standards has been made wherever possible. In those areas where the standards do not fully address the subject, published references and papers were consulted, established experts were contacted and sometimes the methods were augmented by the author's personal research and experiments.

STANDARDS

ANSI CGATS.4-1993, *Graphic technology – Graphic arts reflection densitometry measurements – Terminology, equations, image elements and procedures.*

ANSI CGATS.5-1993, *Graphic technology – Spectral measurement and colorimetric computation for graphic arts images.*

ANSI CGATS.17-2005, *Graphic technology – Exchange format for color and process control data using XML or ASCII text.*

ANSI/IES TM-30-18, *IES Method for Evaluating Light Source Color Rendition.*

ANSI NEMA ANSLG C78.377-2008, *Specifications for the Chromaticity of Solid State Lighting Products.*

ASTM E 308-01, *Standard Practice for Computing the Colors of Objects by Using the CIE System.*

ASTM E 1708-95, *Standard Practice for Electronic Interchange of Color and Appearance Data.*

CIE 13.3-1995, *Method of Measuring and Specifying Colour Rendering Properties of Light Sources*, ISBN 978-3-900-734-57-2.

CIE 15:2004, 3rd Edition, *Colorimetry*, ISBN 3-901-906-33-9.

CIE 015:2018, 4th Edition, *Colorimetry*, ISBN 9783-902842-13-8.

CIE 18.2:1983, *The Basis of Physical Photometry.*

CIE 51.2:1999, *A Method for Assessing the Quality of Daylight Simulators for Colorimetry*, ISBN 3-901-906-03-7

CIE 160:2004, *A Review of Chromatic Adaptation Transforms.*

CIE 167:2005, *Recommended Practice for Tabulating Spectral Data for Use in Colour Computations*, ISBN 3-901-906-41-X.

CIE 175:2006, *A Framework for the Measurement of Visual Appearance*, ISBN 3-901-906-52-5.

CIE 177:2007, *Colour Rendering of White LED Light Sources*, ISBN 978-3-902842-61-9.

CIE 224:2017, *CIE 2017 Colour Fidelity Index for accurate scientific use*, ISBN 978-3-901-906-57-2.

CIE S 001, *Colorimetric Illuminants*.

CIE S 002, *Colorimetric Observers*.

ISO/CD 5-3 2002, *Photography and graphic technology – Density measurements – Part 3: Spectral conditions*.

ISO 8601, *International Standard Date and Time Notation*.

ISO 13655:1996(E), *Graphic technology — Spectral measurement and colorimetric computation for graphic arts images*.

ISO/TR 16066:2003, *Graphic technology—Standard object colour spectra database for colour reproduction evaluation (SOCS)*.

BOOKS

Berger-Schunn, A., *Practical Color Measurement: A Primer for the Beginner, A Reminder for the Expert*, John Wiley & Sons, Inc., New York, 1994, ISBN 0-471-00417-0.

Berns, R. S., *Billmeyer and Saltzman's Principles of Color Technology, Fourth Edition*, John Wiley & Sons, Inc., New York, 2000, ISBN 0-471-19459-X.

Cleveland, W. S., *The Elements of Graphing Data, Revised Edition*, Hobart Press, Summit, New Jersey, 1994, ISBN 0-9634884-1-4.

Fairchild, M. D., *Color Appearance Models, Second Edition*, John Wiley & Sons, Ltd., Chichester, 2005, ISBN 0-470-01216-1.

Hunt, R. W. G. and Pointer, M. R., *Measuring Colour, Fourth Edition*, John Wiley & Sons, Ltd., United Kingdom, 2011, ISBN 978-1-119-97537-3.

Hunt, R. W. G., *The Reproduction of Colour, Fifth Edition*, Fountain Press, England, 1995, ISBN 0-86343-381-2.

Hunter, R. S. and Harold, R. W., *The Measurement of Appearance*, Second Edition, John Wiley & Sons, Inc., New York, 1987, ISBN 0-471-83006-2.

Judd, D. B. and Wyszecki, R. G., *Color in Business, Science and Industry*, Third Edition, John Wiley & Sons, New York, 1975, ISBN 0-471-45212-2.

Kang, H. R., *Computational Color Technology*, SPIE Press, Bellingham, 2006, ISBN 0-8194-6119-9.

MacAdam, D. L., *Color Measurement: Theme and Variations*, Second Revised Edition, Springer-Verlag, Berlin, 1985, ISBN 0-387-10773-8.

Wright, W. D., *The Measurement of Colour*, Fourth Edition, Van Nostrand Reinhold Company, New York, 1971.

Wyszecki, R. G. and Stiles, W. S., *Color Science: Concepts and Methods, Quantitative Data and Formulae*, Second Edition, John Wiley & Sons, Inc., New York, 1982, ISBN 0-471-02106-7.

PAPERS

Li, C., Luo, M. R., Rigg, B. and Hunt, R. W. G., *CMC 2000 Chromatic Adaptation Transform: CMCCAT2000*, *Color Research and Application*, Vol. 27, No. 1, February 2002, pages 49-58.

Myers, R. D., *LCD Monitors and Spectrometers, an Interesting Problem*, https://chromaxion.com/information/lcd_spectro.html. Last accessed 2020-07-02.

Sharma, G, Wu, W., Dalal, E., *The CIEDE2000 Color-Difference Formula: Implementation Notes, Supplementary Test Data, and Mathematical Observations.*

Stokes, M. and Brill, M., *Efficient Computation of ΔH^*_{ab}* , *Color Research and Application*, Vol. 17, No. 6, December 1992, pages 410-411.